



MAGNETO GEOMETRIC APPLICATIONS



45, DOWANHILL ROAD — CATFORD — LONDON SE6 1SX — ENGLAND

GLOSSARY OF ABBREVIATIONS USED WITH
MAGNETO GEOMETRIC APPLICATION PRINCIPLES
AND PROTOCOL

M G A	Magneto geometric applications
C N S	Central nervous system
S N S	Sympathetic nervous system
P S M S	Para-sympathetic nervous system
G I TRACT	Gastro-intestinal tract
N D P F	No detectable Prior Factor
SOLAR P	Solar plexus chakra
ALTA M	Alta Major chakra
WITNESS	Sample of patient's hair, blood spot, urine sample
G T C	Group Treatment Card

INSTRUMENTATION AVAILABLE USING
M.G.A. PRINCIPLES WITH EXPLANATION FOR
THEIR USAGE

- 1 MK3 Potency Simulator
- 2 Extended Range Potency Simulator
- 3 Extended Range 4 - Section Multiple Simulator
- 4 Potency Preparer
- 5 Extended Range Potency Preparer
- 6 Interrupter
- 7 Rae Analyser (including charts and cards)
- 8 Twin Instrument
- 9 Triple Instrument
- 10 Test Case Example

INTRODUCTION TO THE WORK AND
DISCOVERIES OF THE LATE MALCOLM RAE
AND THE PRINCIPLES OF M.G.A.

- 1 That all living organisms emit a measurable vibration which can be interpreted by a trained Dowser and documented for future comparisons.
- 2 That all homoeopathic remedies, whether made by succussion/dilution methods, or M.G.A. principles emit measurable energies which can be documented for comparison against physical or subtle anatomy energies.
- 3 That in the concept of Homoeopathy Dr. Hahnemann gave to the world an extremely effective system of therapy, which has survived the test of time incredibly well, even though time has been very unkind to the therapy.
- 4 That by the Dowsing faculty it is possible, by using M.G.A. principles, to prepare simulator cards of gems, colour, bio-chemistry, vitamins, combination remedies and actual rate systems for all known organs, systems and cellular body functions, as well as the energies of the subtle anatomy and planetary influences.
- 5 That these subtle energies can be used by the trained Dowser to analyse and treat the physical or subtle anatomy.
- 6 That by the use of energies and patterns, remedies may be reproduced on a repeatable basis with instruments for oral use, or by projection over a suitable witness.
- 7 That the use of the Dowsing sense over an instrument using patterns will reveal imbalances or harmony when compared with the Patient,s witness, and enable remedies to be selected to treat the Patients conditions.
- 8 One important factor to remember is that the M.G.A. method of potentisation cannot produce substance. Remedies prepared by this method, of potencies less than 12c will differ only fractionally from the succussion/dilution prepared counterparts in that they will contain no residue of the substance from which they are prepared.

- 9 That remedies can be prepared such as Oxygen M, sunlight or gems etc, which could not normally be prepared by the succussion/dilution method.



Before discussing the instruments it is essential to know the principles of M.G.A. using the card system, based on the late Malcolm Rae's paper called Homoeopathy up to Date. Dowsers frequently use a 100 cm rule, (see figure 1) along which to measure the "potency energy" of a sample of a remedy. With the sample located at the "Zero" end of the rule, they move the pendulum along the rule from left to right, noting the point at which the pendulum swings exactly at right angles to the rule. This point indicates a relative potency energy.

It is suggested that the point of balance thus detected is, in fact, the "boundary" between the remedy's local field, and a component of the earth's magnetic field, and this view was to some extent corroborated by the observation that measurements made with the rule differently orientated in relation to the terrestrial field yielded different balance points.

This led to a series of measurements being made in respect of several different remedies, using the remedy vial as the central point, and finding the balance point along the rule, with it pointing in turn to each of the Cardinal and half Cardinal points of the compass. The results of these measurements were then plotted on polar graph paper, and the adjacent points joined by straight lines to form a geometric pattern related to each remedy. Each point was found to be solely related to one remedy.

If the interaction of the remedy's energy field with the earth's field resulted in a pattern related to the remedy, it seemed not unlikely that the interaction of the earth's field and the pattern could be used to create a replica of the remedy: and the experiments proved this to be the case.

An interesting point then discovered was that the alignment of the pattern with the orientation in which it has been drawn resulted in the replica being of a very high potency (theoretically, infinite potency), whilst the greater degree of misalignment the lower the potency replicated. From this, a scale was developed, against which to set the pattern to the required

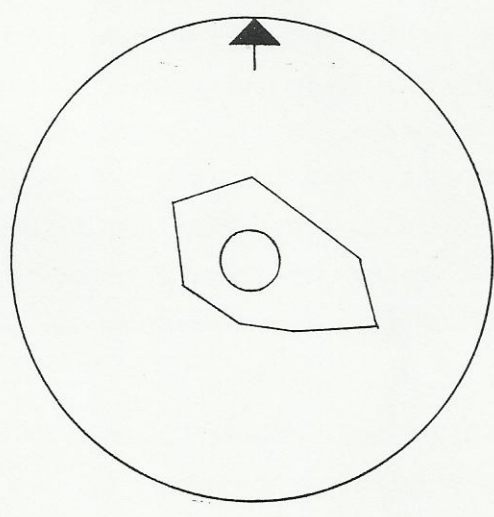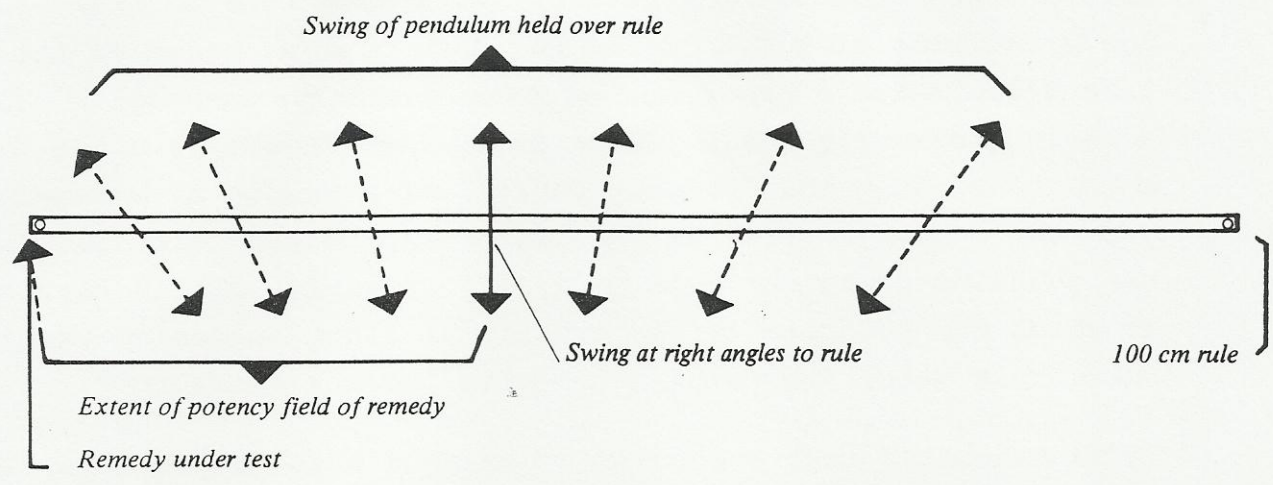

*Circular potency simulator card
representing Argentum Nitricum*

8

potency. At that time - 1966 - a number of patterns related to remedies were prepared, each drawn on a circular disc orientated North - South, and a few experimental instruments were constructed. The remedy discs were similar to those depicted as figure 2, and the "instruments" approximately as shown in figure 3.

Dowsing tests made with a number of remedies prepared in this manner indicated them to be matched with conventionally prepared remedies: and their effects upon those taking them appeared to be similar: and, in fact, they were encouraging enough to stimulate the consideration of a new instrument. Amongst a number of obvious shortcomings in the initial design, it seemed imperative that the following should be eliminated:-

- (a) Circular remedy cards would be costly to produce, inconvenient to store, and would restrict the diameter of the vial used which must be the same as the hole in the card.
- (b) the use of the earth's field as an energiser meant that the instrument must be correctly orientated, for were it misorientated, it would yield a potency other than indicated on the scale.

To overcome the former, experiments were undertaken to discover whether the influence of the energised pattern could be guided along a wire from the centre of the drawing to the base of a cylindrical container to which a vial could be placed. These experiments confirmed that this could be done, with the result that the pattern could be located vertically, and thus be removed from the relevant effects of the earth's field. See figure 4

Further experiments showed that the earth's field could be replaced by that of a small permanent magnet: and hence it became possible to enclose the instruments in a suitable case. During the investigations it had been discovered that a card bearing a circle, magnetically energised, would erase the pattern from a potentised medium placed within the circle: and also that it would erase the potency energy from a conventionally prepared Homoeopathic remedy. The potency could be restored to the conventionally prepared remedy by succussion, without the addition of further substance: whereas all record of the

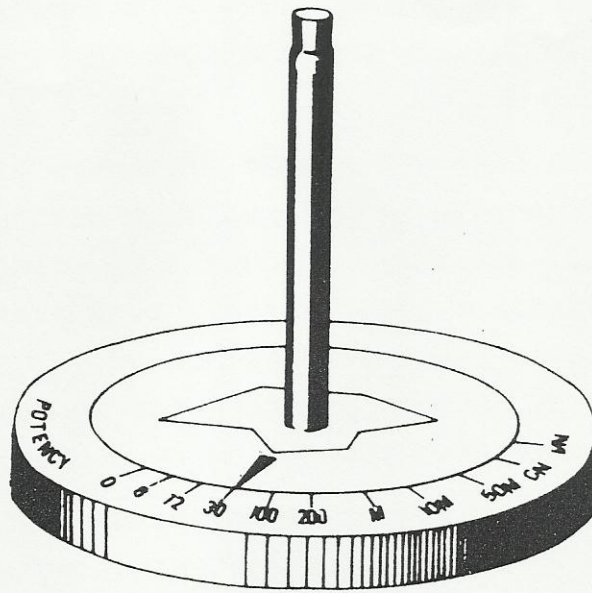


Fig. 3

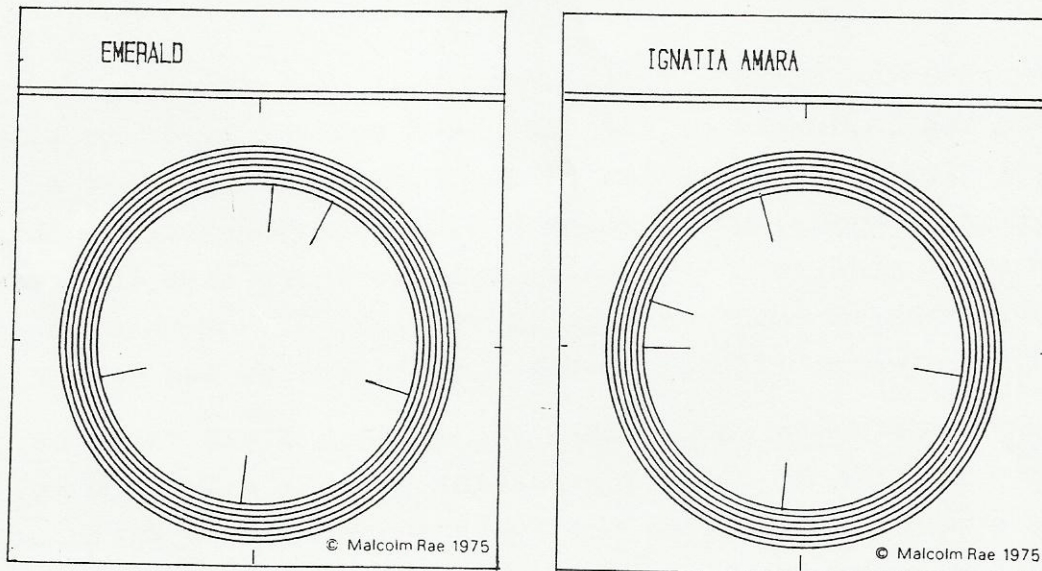


Fig. 4

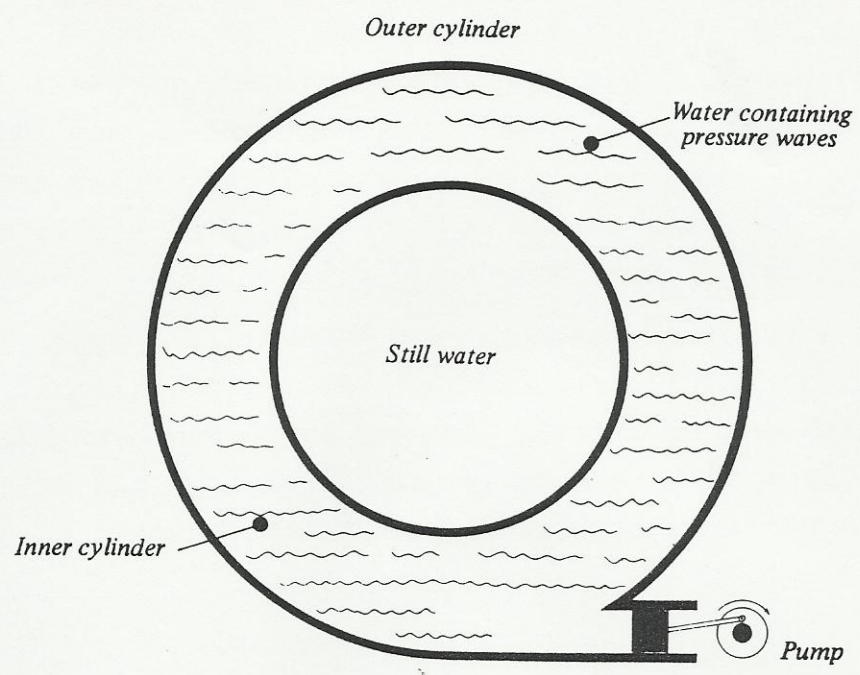


Fig. 5

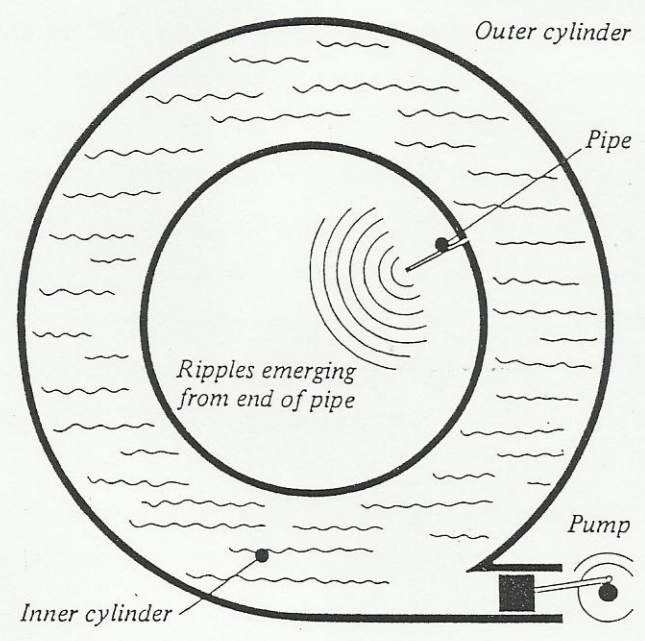


Fig. 6

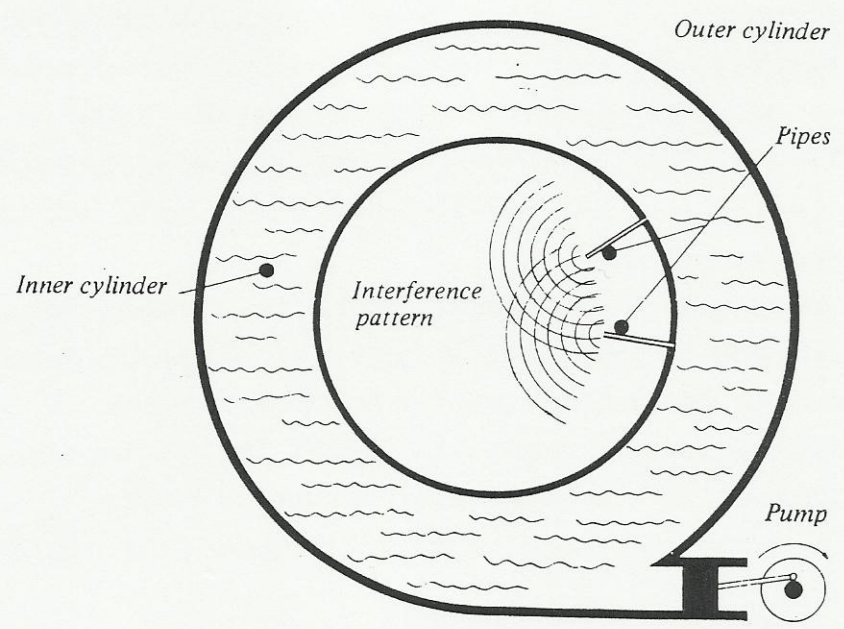


Fig. 7

remedy was erased from a magneto-geometrically prepared remedy. It was therefore decided to incorporate a "neutraliser" in the form of a magnetically energised circle, which could be switched to the base of the cylindrical vial container, which became known as the "well".

Energised by a permanent magnet, the vertically located pattern resulted in the production of energy of "infinite potency", which due to circuit losses, was reduced to slightly above 10 mm. From this varying amounts of energy had to be drawn off, to yield the required potency at the base of the instrument's well.

To recap briefly the following principles apply to all M.G.A. instruments and their usage.

- A 1 The specific characteristics of any substance may be expressed numerically as a group of ratios, or represented by a pattern geometrically expressing ratios.
- 2 The appropriate application of magnetism to a geometric expression of a substance creates an influence which will be recorded by water, whether free, or as a component of any other substance, which lies within that influence.
- 3 The appropriate application of magnetism to any substance will create an influence which will be recorded by water within that influence.
- 4 The water influenced is the equivalent in its effect upon a living organism, of a conventionally prepared homoeopathic medicine.

B APPLICATION OF PRINCIPLE TO INSTRUMENTS

- 1 Instruments designed to employ this principle have been in use for several years, and over 3,000 are currently in use.
- 2 A stock of some 5,000 geometric patterns, on cards measuring 75mm x 65mm, includes those representing almost every well-known homoeopathic medicine, and many hundreds of less-known remedies.
- 3 The basic structure of the instruments is a small box equipped with one or more slots into which remedy cards fit, one or more calibrated controls on which the required potency(ies) is/are set, and a "well" into which the phial containing the distilled water or other substance (usually sac lac) to be potentised, is placed.

- 4 Each instrument is also fitted with two sockets: one to accept a single plug enabling it to be connected to a further instrument; and the other to accept a jack plug connected to a suitable pulse generator (interrupter) to convert the instrument into a projection instrument.
- 5 Care should be taken to ensure that only cards purchased from Magneto Geometric Applications are used in the instruments. There are no agents or other suppliers and are only available from the London address shown at the front of this manual. The cards are distinguishable by the name "Malcolm Rae" on the front and by either of the two addresses or the MGA logo on the reverse as shown below.

MALCOLM RAE,
47, Lee High Road,
Lewisham,
London, SE13 5NS,
England.

Telephone: 01-852 8292

Malcolm Rae
3 The Hermitage
Westwood Park
Forest Hill
London SE23 3RU
England

Tel: 01-699 6604

MAGNETO
GEOMETRIC
APPLICATIONS



THE MARK 111 POTENCY SIMULATOR as illustrated see figure 8

A To prepare a Potency:-

(It is imperative that the following sequence of operations is observed)

- 1 With the instrument positioned with the slot at the end furthest from the operator, insert the card for the required remedy in the slot, with the name upwards and facing the operator.
- 2 Set the pointer of the potency control to the required potency.
- 3 Place the medium to be potentised either directly in the well of the instrument, or in a previously neutralised phial in the well of the instrument. IMPORTANT: only cylindrical phials should be used.
- 4 If sac lac is the medium to be potentised, the pilules should be moistened prior to placing them in the simulator well. This is because the potentising process depends upon the presence of moisture in the medium to be potentised and although sac lac pilules contain some water, it is advisable to moisten them sufficiently for them to appear shiny, but not to cause them to start dissolving. Because it has a more rapid evaporation rate than water it is preferable to moisten with thirty per cent (or thereabouts) alcohol.
Gin or Vodka will meet this requirement without discolouring the sac lac.
For small quantities of pilules, it is convenient to use a short length of wire, which when dipped into the liquid used and then withdrawn, will form a small globule on its end. The volume of the globule depends upon the thickness of the wire and the depth to which it is lowered in the liquid. For larger quantities of pilules, a dropping bottle is more suitable.
In either case the pilules should be thoroughly shaken after the liquid has been added, in order to spread it as evenly as possible over their surfaces.
- 5 Leave the medium in the well for a minimum of one minute if water is being potentised, and for a minimum of six minutes

if sac lac is the medium.

- 6 The medium is fully potentised on termination of these times, and will not be affected by additional time in the instrument.

IMPORTANT: The potentised medium must be removed from the instrument before the remedy card is removed- otherwise the medium will be subjected to neutralisation.

B To Neutralise a Potency:-

- 1 Ensure that no remedy card is in the slot.
- 2 Set the potency control at 10MM.
- 3 Place the medium to be neutralised either directly in the well of the instrument, or in a phial in the well of the instrument. IMPORTANT: only cylindrical phials should be used.
- 4 Leave for a minimum of one minute if water, and a minimum of six minutes if sac lac.
- 5 The medium will then be neutral and ready to accept a further potentisation.

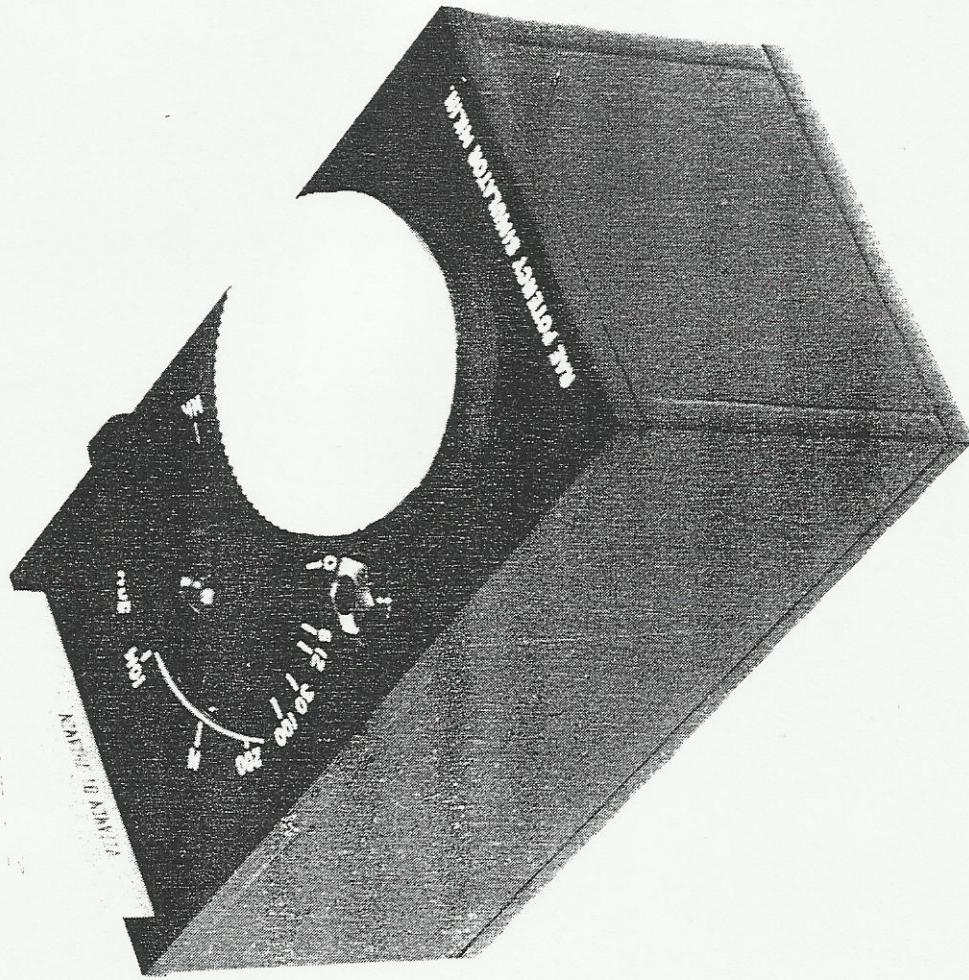


Fig. 8 The Homeopathic Potency Simulator

THE EXTENDED RANGE POTENCY SIMULATOR as illustrated see figure 9

Although a magneto-geometrically prepared remedy of potency below 12C does not exactly match its succussion-dilution prepared namesake, insofar as the former contains no material, whilst the latter contains traces of material, the experience of many users has proved low-potency magneto-geometrically prepared remedies to be effective.

The Extended Range Potency Simulator employs a digital dial, calibrated from "000" to "1000" (though the "1" of the "1000" position does not appear on the dial), to provide a scale length approximately 12 times the length of that of the Mark 111. Since it is not possible to calibrate this type of dial directly in potencies, a conversion graph is necessary.

INSTRUCTIONS - THE EXTENDED RANGE POTENCY SIMULATOR:-

All instructions for the Extended Range Potency Simulator are identical with those for the Mark 111 with the exception of (2)

- 1 Select the graph down the right-hand side of which the required potency appears.
- 2 Locate the required potency and follow the horizontal line from it to the left until it meets the curve of the graph.
- 3 From the point where it meets the curve of the graph, follow the vertical line down the scale along the bottom edge of the graph, and read off the instrument's dial setting.
- 4 On graph "A", range 1x to 12x, each small division along the base line represents 5 degrees.
On graph "B", range 1c to 1M, each small division along the base line represents 10 degrees.
- 5 A small lever projecting from the front edge of the dial will lock the setting at any number.
- 6 It is important to avoid forcing the dial beyond either the maximum or the minimum settings; or trying to turn the knob when the lock has been applied, as the mechanism may be damaged by so doing.


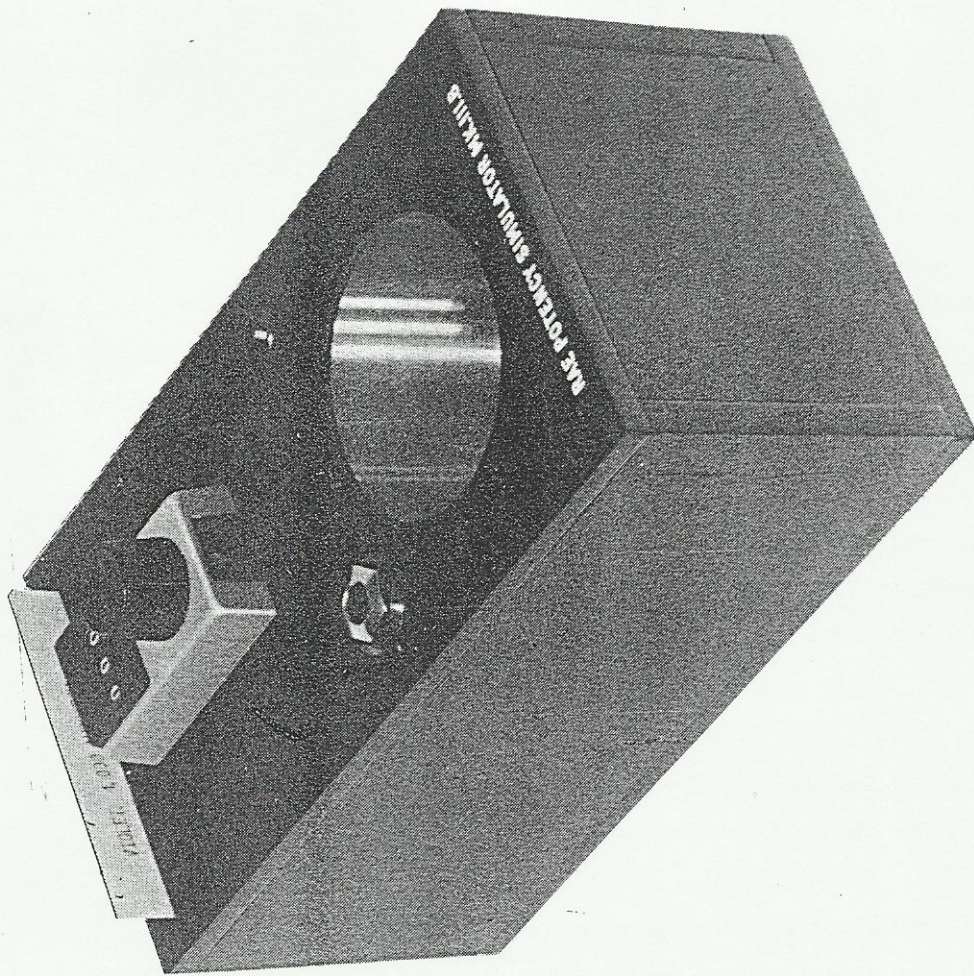


Fig. 9 The Extended Range Homeopathic Potency Simulator

GRAPH A

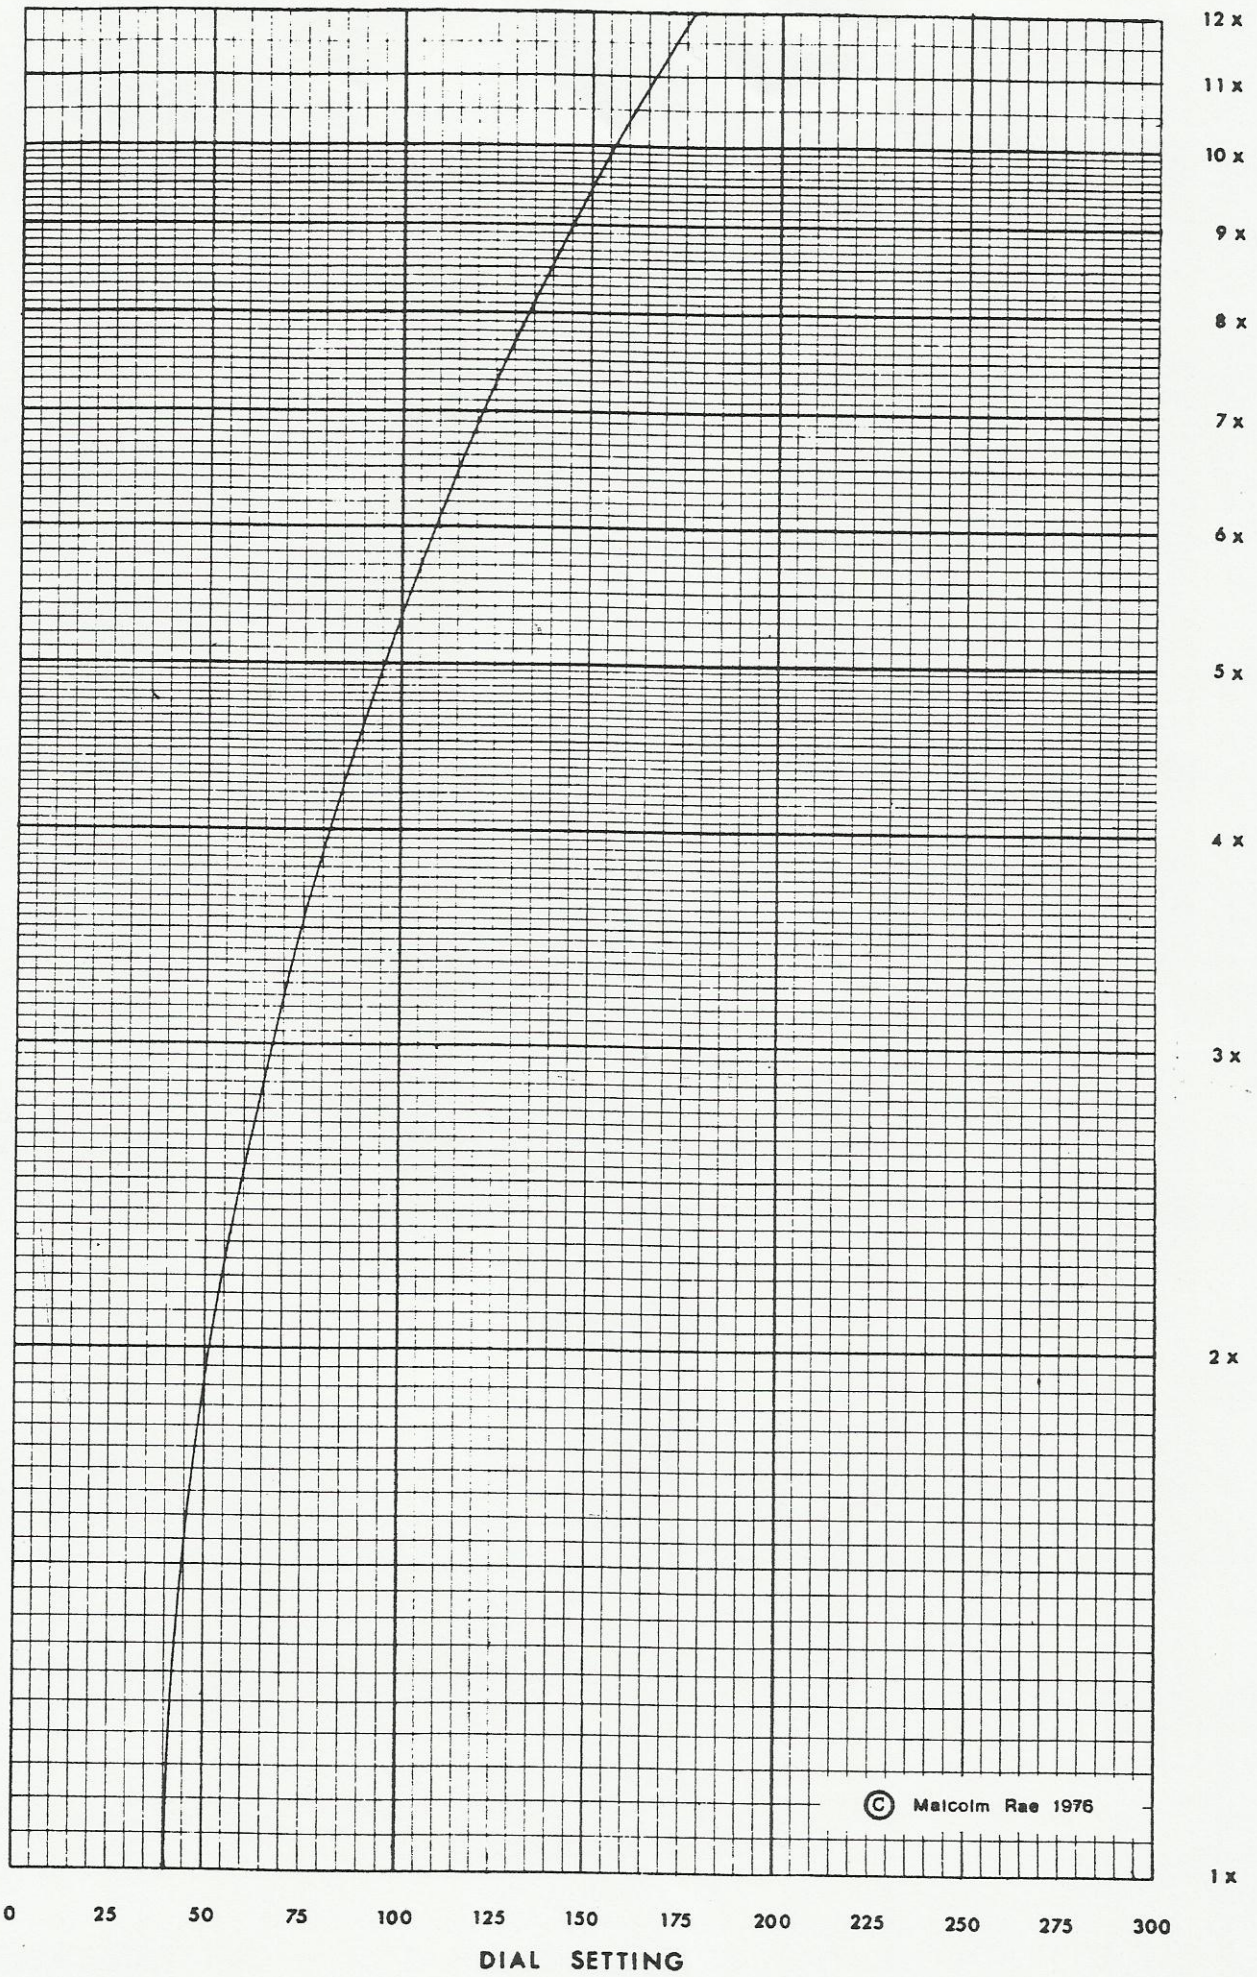


© Malcolm Rae 1976

POTENCY

DIAL SETTING

RAE EXTENDED RANGE POTENCY SIMULATOR — SETTING CHART

Fig 10

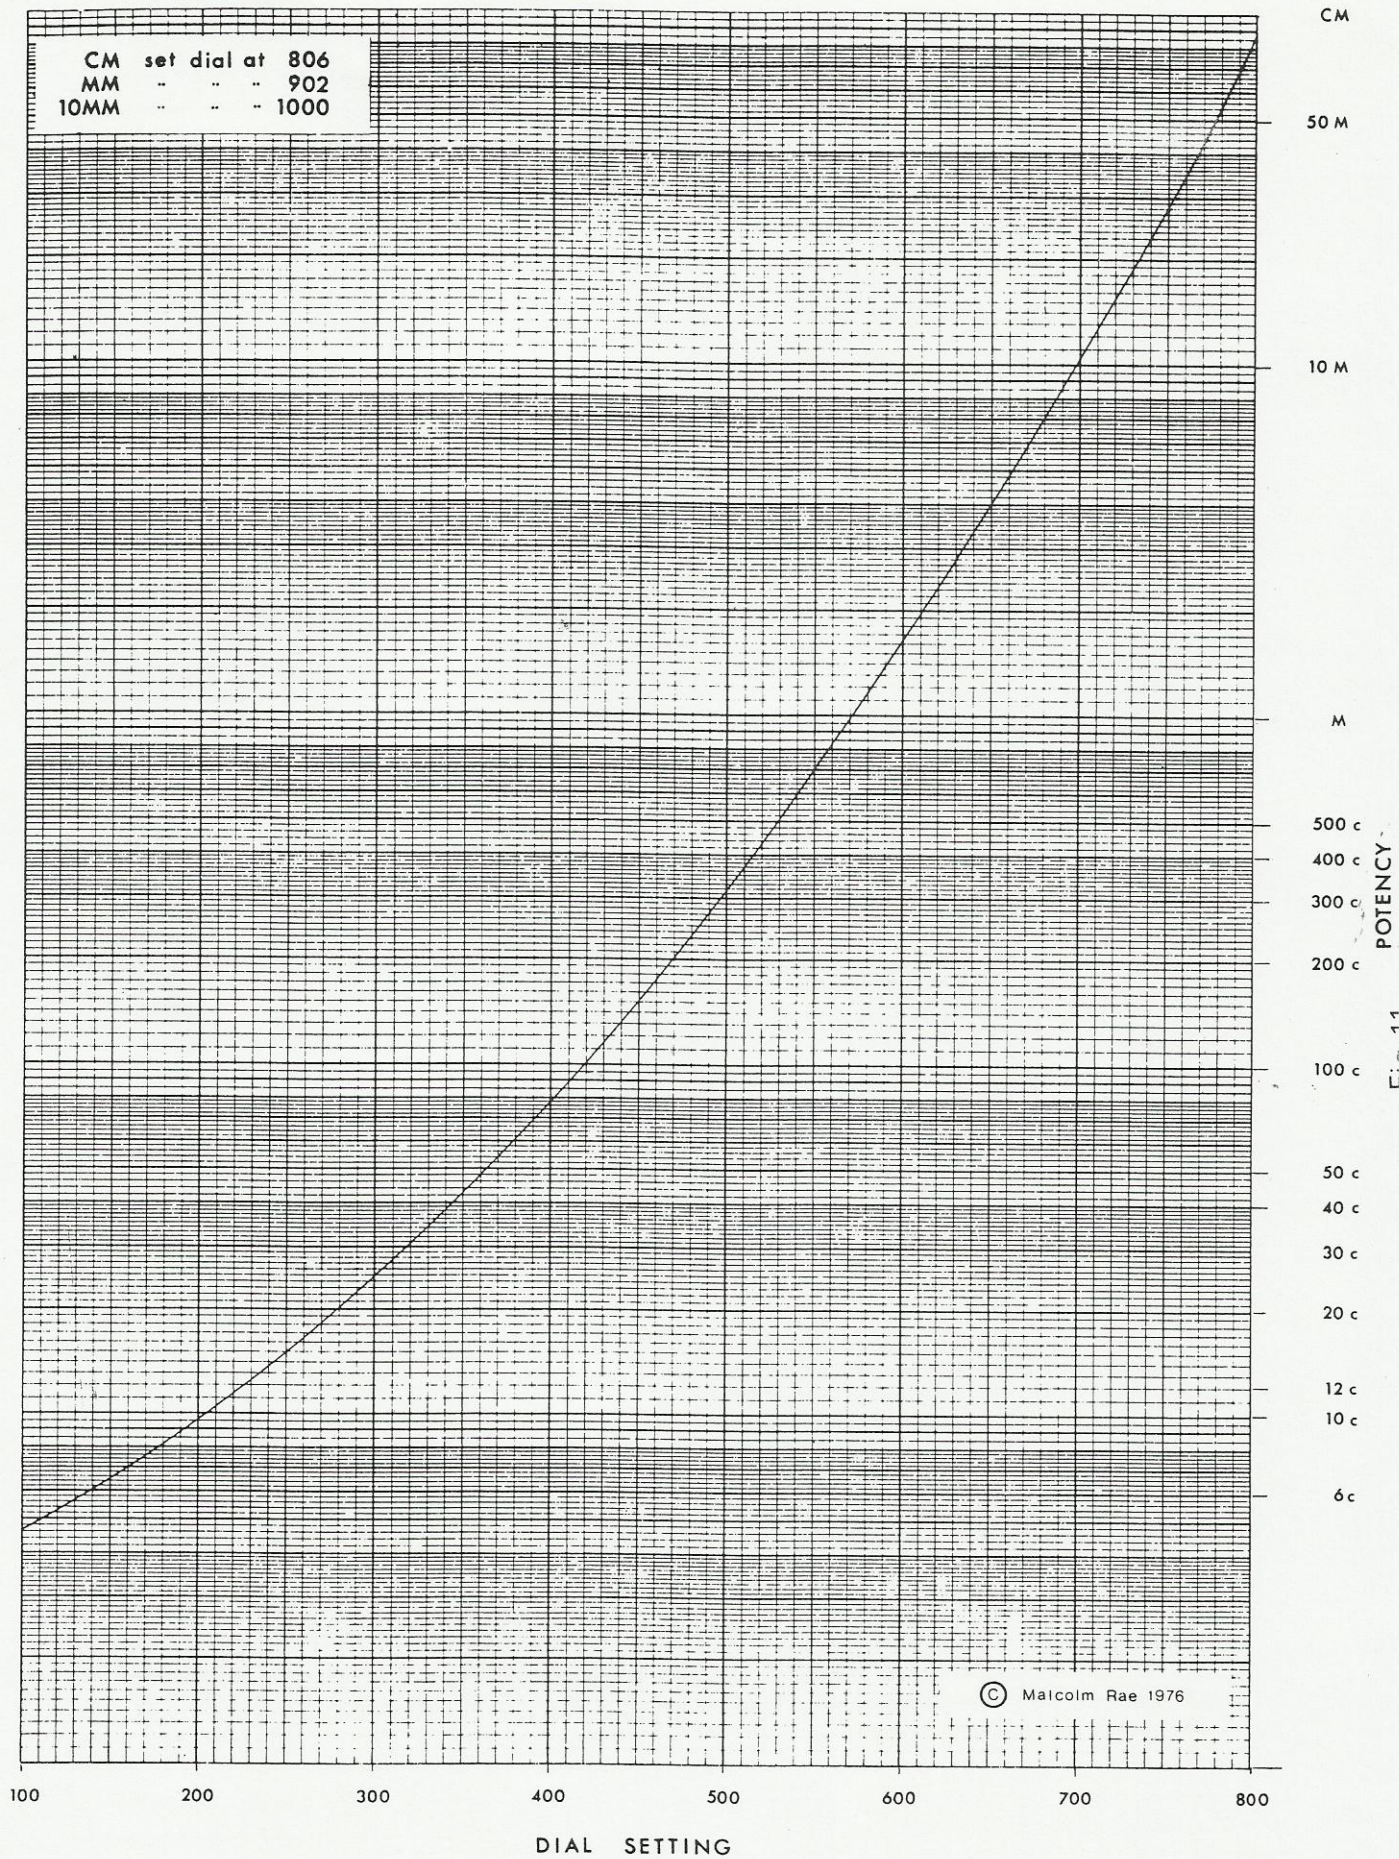

RAE EXTENDED RANGE POTENCY SIMULATOR — SETTING CHART

THE EXTENDED RANGE 4 - SECTION MULTIPLE REMEDY POTENCY SIMULATOR:

It is not possible to prepare a multiple remedy consisting of more than one component by potentiating the medium with the card for each component in turn, because each potentiation partially erases the effects of its predecessors. It can be done by potentiating an equal volume of water with the card for each component of the remedy and mixing the results. However, this is a time - consuming process, and the 4-section Multiple Simulator was designed to solve the problem. It can prepare a remedy with one, two, three or four components in one operation, with each component at the same or different potencies.

INSTRUCTIONS:

This instrument is operated in exactly the same way as the Extended Range Potency Simulator.

- 1 Single remedies may be prepared in the instrument by having all but one of the switches in the "OFF" position (ie, switch lever pointing towards the digital dial), setting the required potency, and inserting the remedy card in the section that is "ON" (ie switch lever pointing away from the digital dial).
- 2 Multiple remedies consisting of up to four components may be prepared by inserting a card for each component in the slot of each section, setting the potency dial of each section to the required potency, and the switch for each section that is in use at the "ON" position.

IMPORTANT: It is essential that switches for all sections not in use are set at "OFF".

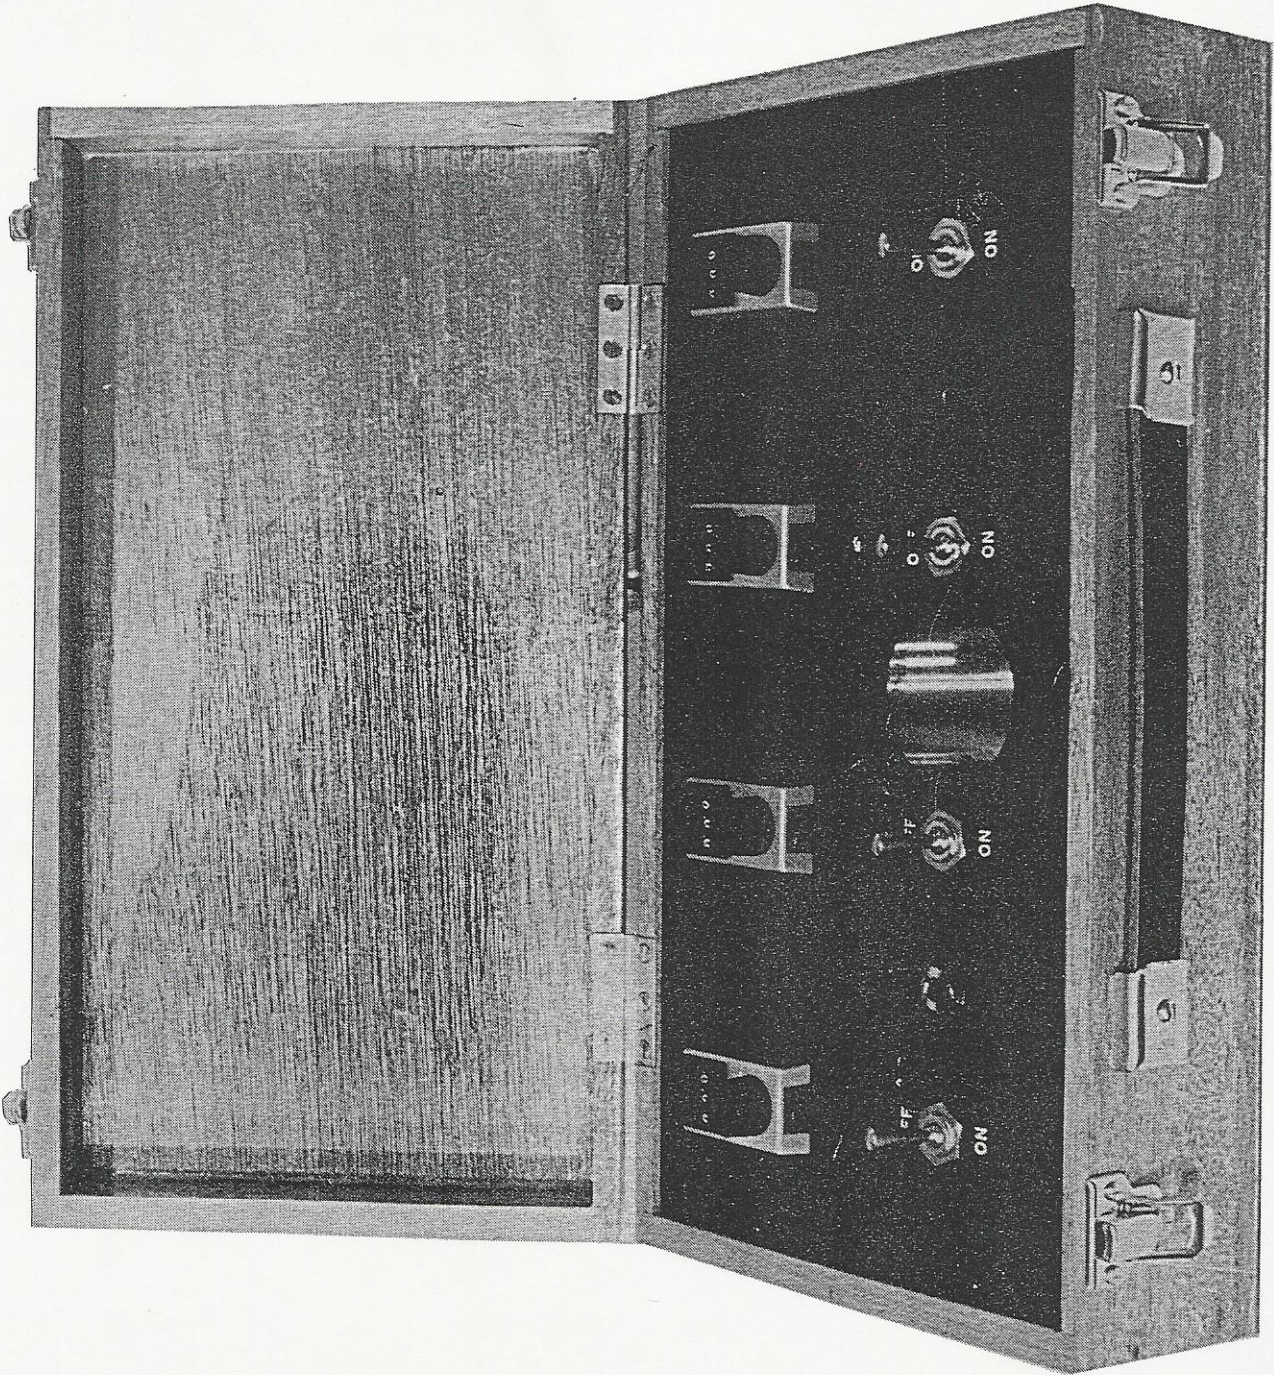


Fig. 12 The Extended Range Multiple Homeopathic Potency Simulator

THE RAE MAGNETIC HOMOEOPATHIC PREPARER as illustrated see figure 10

This instrument differs from those previously described, and is, in fact, complementary to them, its purpose being to prepare, in a single operation, with-out succussion, dilution, mechanical agitation, or the application of any external source of energy, the following:-

- 1 any homoeopathic potency from a sample of any substance or combination of substances.
- 2 any homoeopathic potency from any other homoeopathic potency of the same substance.

INSTRUCTIONS:

IT IS IMPERATIVE THAT THE FOLLOWING SEQUENCE OF OPERATIONS IS OBSERVED:-

- 1 To prepare a potency from a sample of any substance:
 - a. Place the sample in the "input well", in a cylindrical phial.
 - b. Set the potency control to the desired potency.
 - c. Place the medium to be potentised (distilled water, moistened sac lac, or aqueous cream etc) in the "output well", in a cylindrical phial of the same substances as that used in the "input well". (i.e. Plastic in both, glass in both etc.)
 - d. Leave for a minimum of 10 minutes. (Time in excess of ten minutes has no additional effect.)
 - e. Remove the potentised medium from the "output well".
 - f. Remove the sample from the "input well".
- 2 To prepare a potency from any other potency of the same substance:-
Place the existing potency in the "input well", and follow the sequence 1. (a) to 1. (f) above.
The potency to be prepared may be higher or lower than that of the existing potency.
- 3
 - a. In neither case is the sample destroyed by the process- but it is raised to a very high potency (above 10MM), and should not, therefore, be held in the hand for more than a few seconds.
 - b. This does not render it unsuitable for use in the preparation of further potencies, but it must not be subsequently

administered orally in the belief that it is unchanged.

- c. Should it be desired to de-potentise a sample of substance, however, this may be done by allowing it to remain in the "output well", with the "inputwell" empty of everything including the cylindrical plastic phial, and the potency control set at 10MM, for a minimum of ten minutes.
- 4 It is, of course, necessary to sterilize the "input" phial immediately after it has contained any infectious or potentially infectious material.

SPECIAL APPLICATIONS:

Since the instrument prepares a potency of every aspect of the contents of the "input" phial, it is especially suitable for the preparation of:-

- 1 Nosodes from patients' blood, urine, sputum, etc.
- 2 Individualistic remedies sometimes required in treating allergies, such as hair from a particular animal, pollen from a particular variety of flower: foodstuffs. etc.
- 3 Potencies of gems, where representation of the therapeutic characteristic extends beyond the chemical composition.
- 4 Potencies of mixtures of substances. (But not potencies of mixtures of different potencies, because the components would all be reduced or expanded to the same potency.)

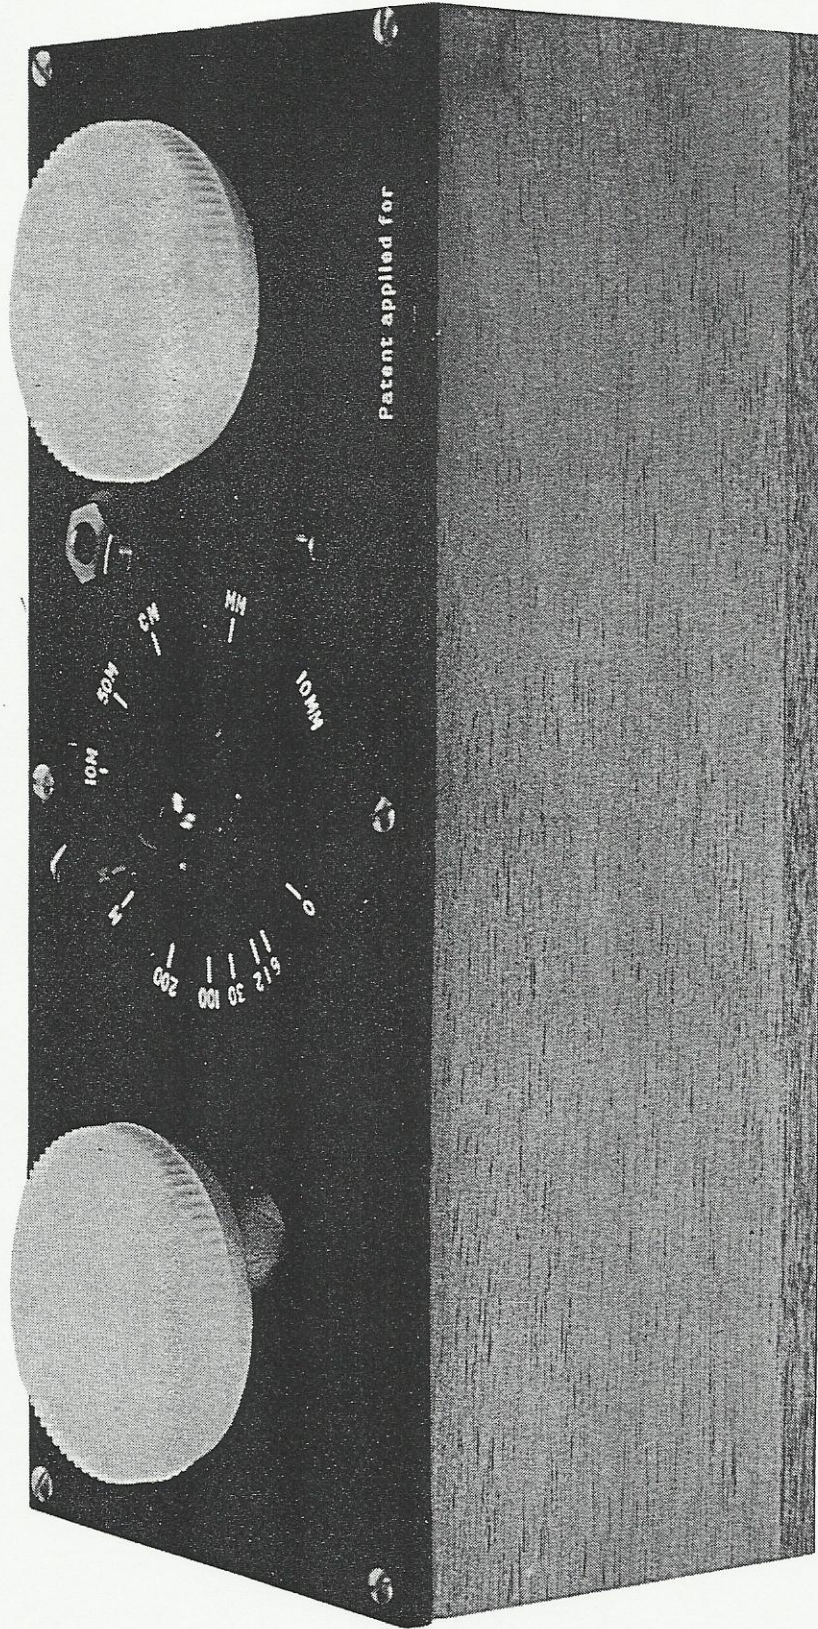


Fig. 13 The Homeopathic Potency Preparer

EXTENDED RANGE POTENCY PREPARER:

Instructions are the same as the Potency Preparer, but use of graphs as in the extended Range Potency Simulator, for selecting potencies of intermediate and lower ranges.

INTERRUPTER:

An electronic interrupter housed in an alloy box, operating from AC mains - either 240 volts 50 cycles or 110 volts 60 cycles, provides the necessary pulsations to convert any of the Rae instruments into projectors from which the remedy may be administered via a sample of the patient's hair.

INTERRUPTER DISTRIBUTION BOX:

A single interrupter will operate several instruments simultaneously, and a small junction box, and four additional leads, each with a jack at either end is all that is needed to enable it to do this.

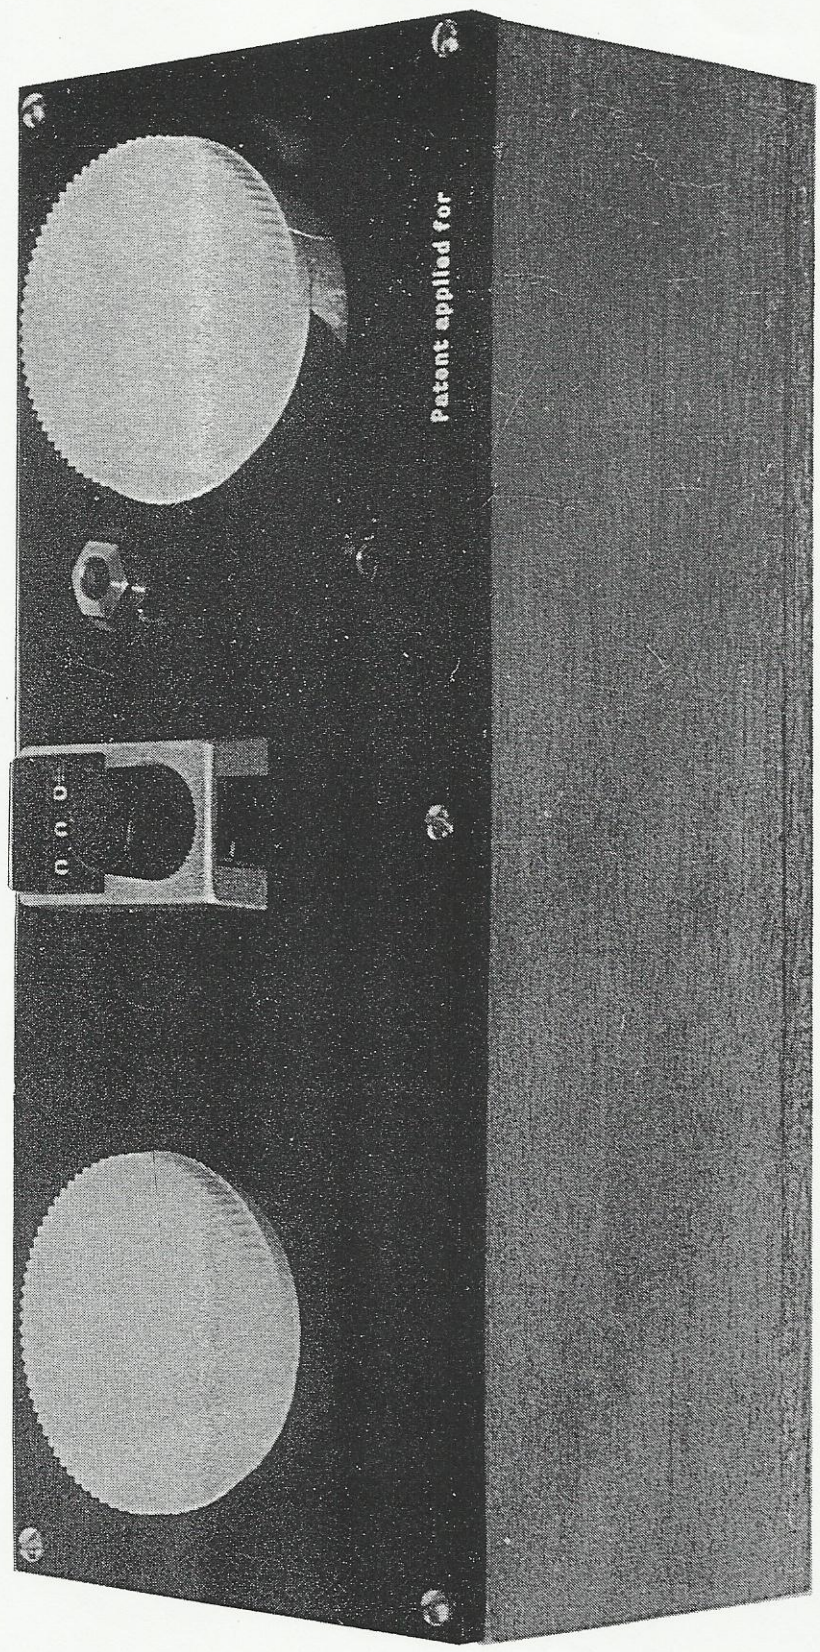


Fig. 14 The Extended Range Homeopathic Potency Preparer

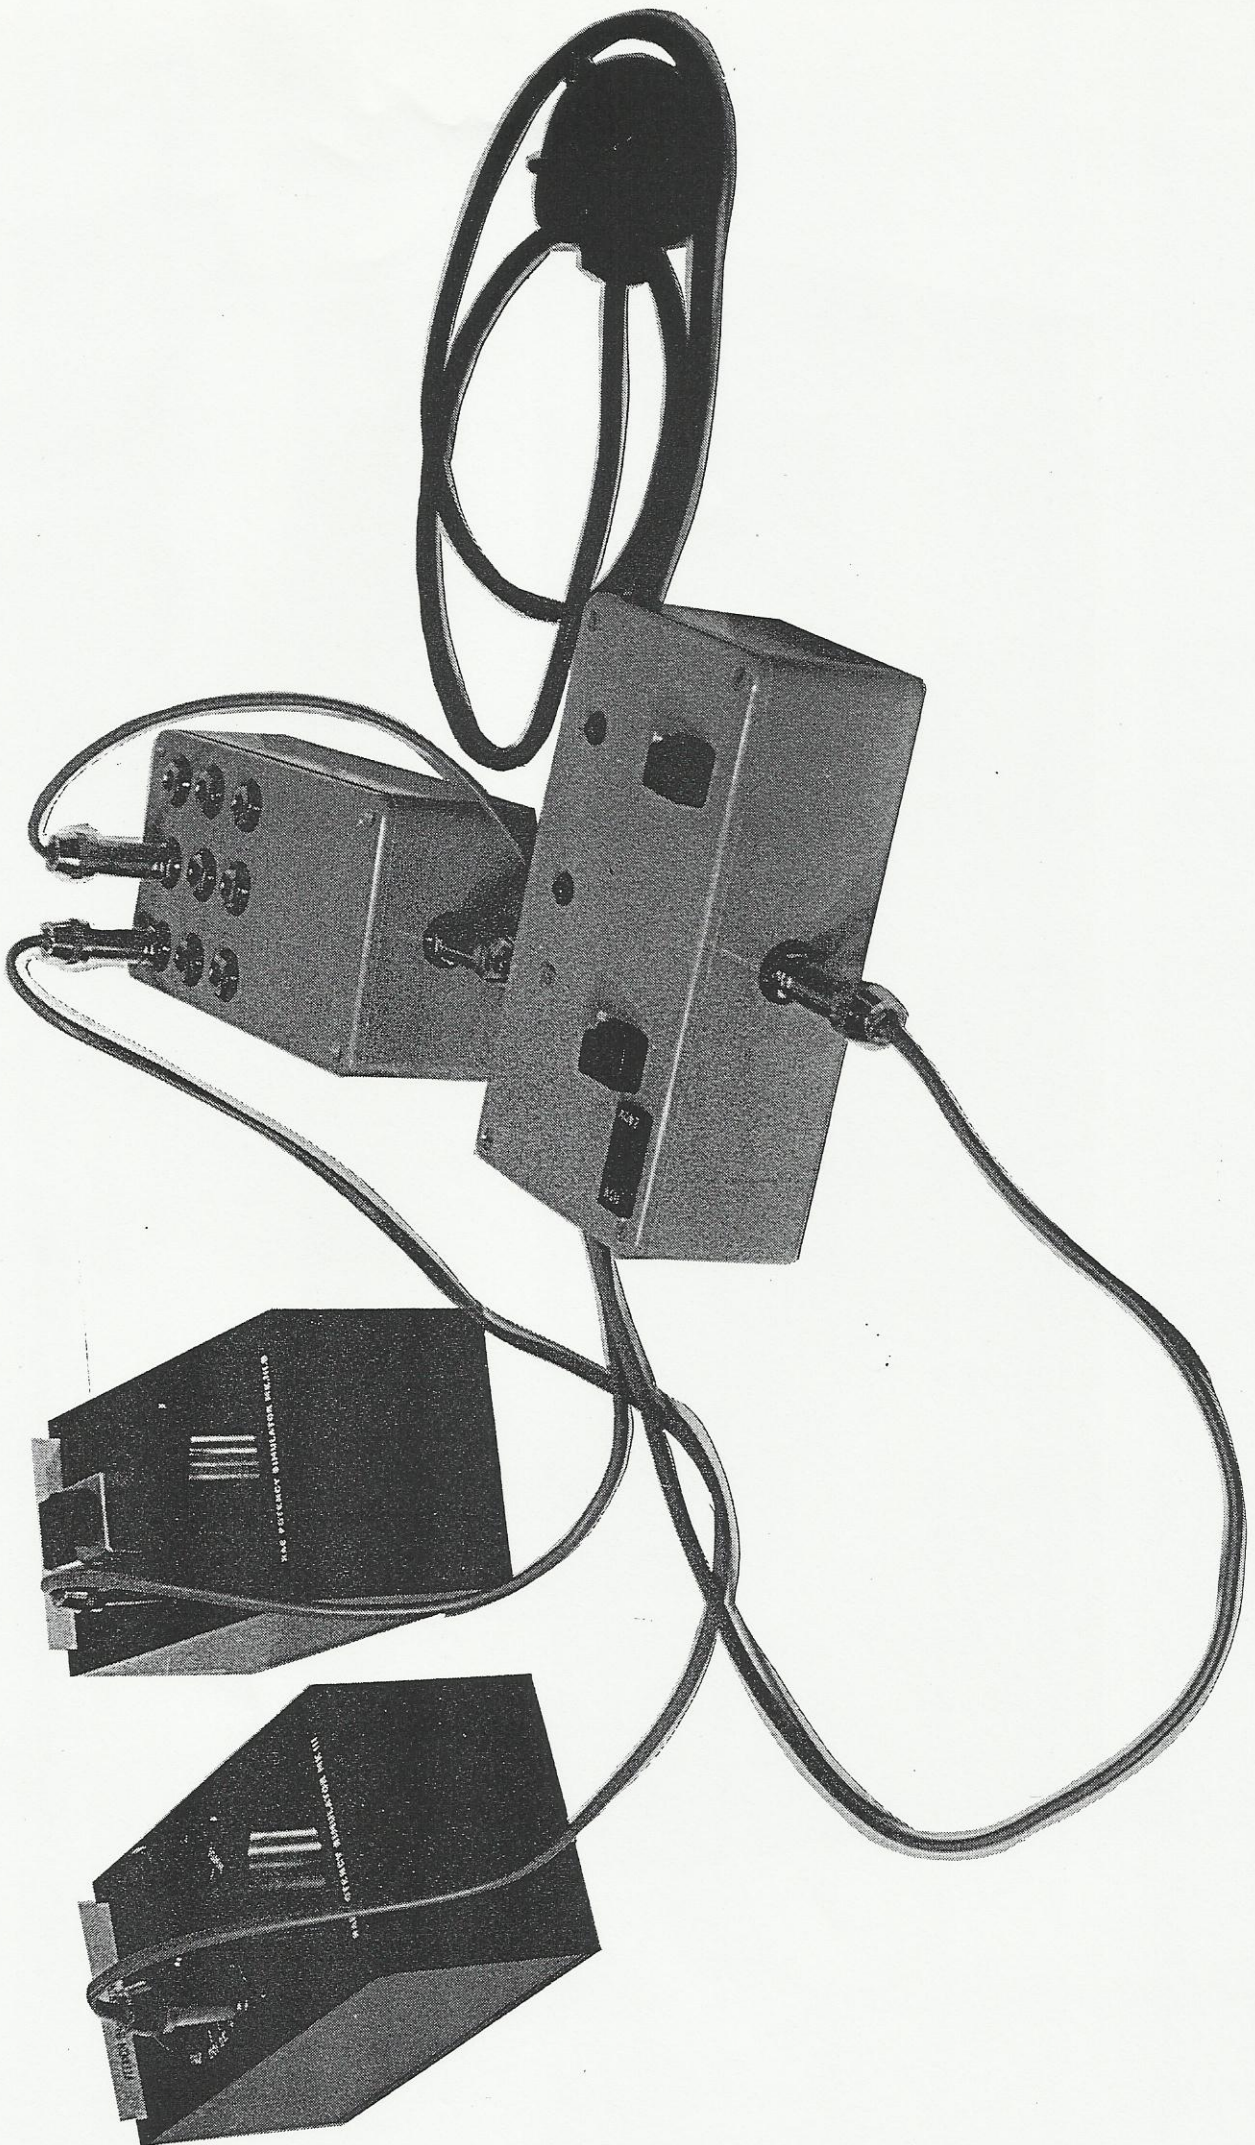


Fig. 15 The Interupter & Junction Box in use

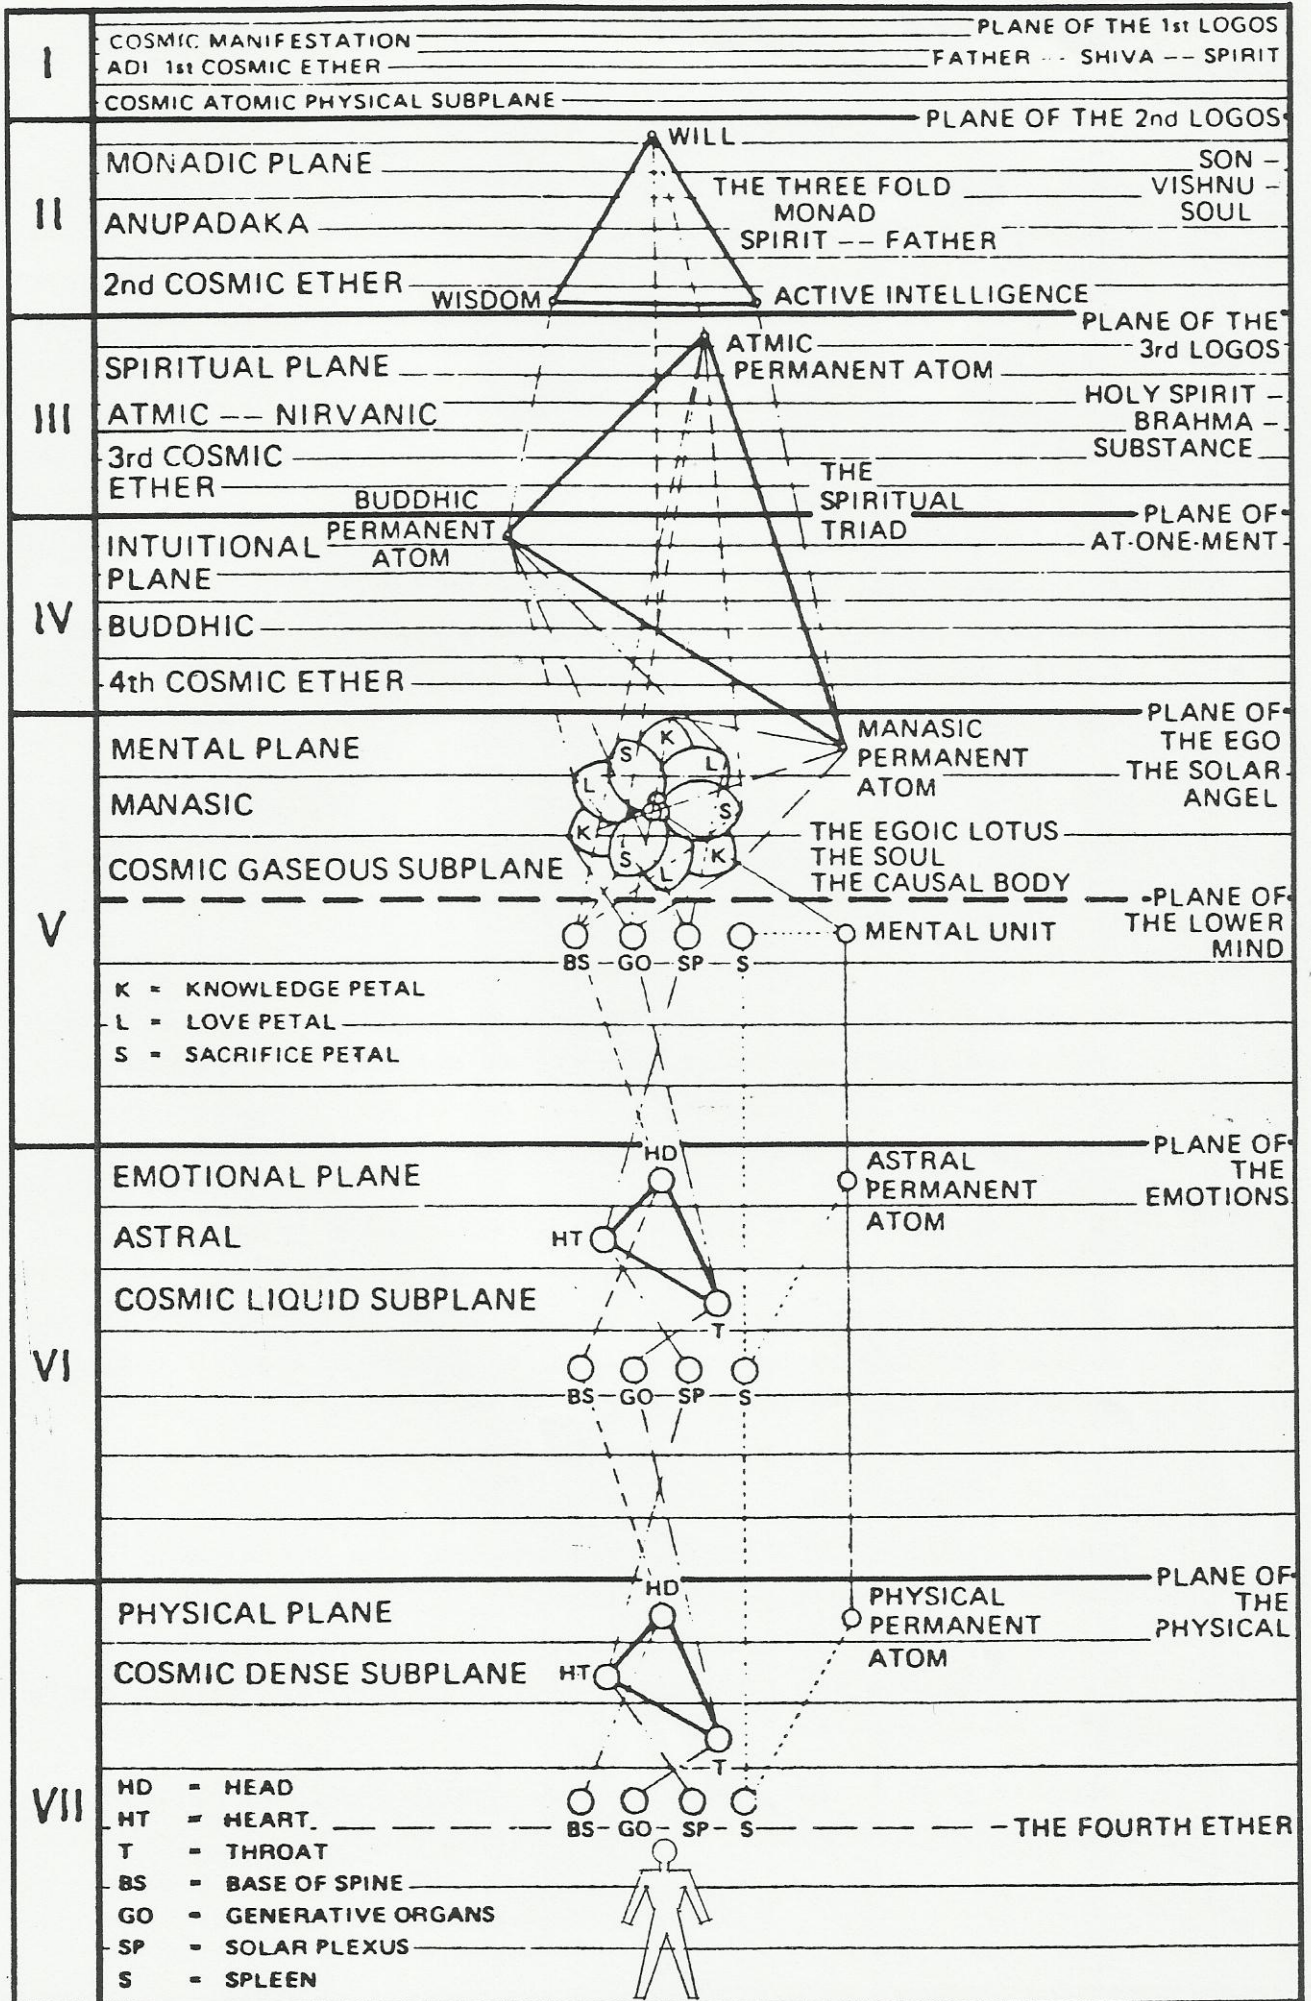


Fig. 16

THE RAE ANALYSER:

PRINCIPLE:-

The instrument employs the now well-tried principle of magneto-geometry - that is, the data is fed into it in the form of cards, representing organs, named diseases, and remedies, and measurements of the patient's condition and remedial requirements are made against these.

The instrument thus defines the information which the operator seeks, and he obtains this by the use of a pendulum over a chart which is connected to the instrument's output.

This is in effect a refinement of the customary use by Dowzers, of a 100cm rule along which to measure the "balance point" between a remedy and a patient's requirement for that remedy; but it is arranged to provide the basis of a rapid and searching analytical system.

IT MUST BE EMPHASISED THAT THE OPERATION OF THIS INSTRUMENT IS DEPENDENT UPON THE PRACTITIONER'S DOWSING SENSITIVITY USING A PENDULUM.

OPERATION

The analyser is extremely flexible in application, and users will undoubtedly develop their individual methods of employing it, nevertheless the following is offered as one effective method, using the Subtle Anatomy Analysis Sheet.

It is important that interested practitioners should be familiar with subtle anatomy principles and have some knowledge of the writing of David Tansley and Alice Bailey on the subject, as the analysis is not restricted to physical anatomy only. (Note Alice Bailey diagram).

Method of Analysis:

Understanding of the following question, and having complete clarity of its full meaning is essential. The questions asked when beginning the analysis of the subtle anatomy are as follows;
First:- What is the "Degree of deviation from functional perfection of"-----

Second:- What is the "Degree of deviation from the patients own soul ray influence that affects optimum functioning of"-----

The patients witness whether a snippet of hair or blood spot is placed between two sticky labels and the patients name and date of birth written on one side. This sample is then placed in the ring marked patients witness, on the Analysis Chart.

The analysis begins with the subtle body, and the card for Mental Body is placed in the location slot with the switch in the "on" position. With the "mean - max" switch at "max" the first question is posed mentally with the pendulum swinging down the line of "0" degrees, "What is the degree of deviation from functional perfection of this patients mental body", watch for the pendulum reaction and read off the degrees of deviation and make a mental note, whilst the pendulum is still swinging, pose the second mental question, "what is the degree of deviation from the patients own soul ray influence that affects optimum functioning of the mental body".

If the pendulum remains at the same degree of deviation as registered by the first question then the conclusion is that the mental body is a treatable area, because the degree of deviation registered is not caused by the patients own soul ray influence, but is from some form of environmental stress or other effects from outside the patients direct control. If, with the second question posed the pendulum returns to "0" then it means that the patient's own soul ray influence is causing the deviation previously recorded i.e. it is normal for this deviation previously recorded to be in existence because there is no deviation from the soul ray influence, therefore the malfunction will be difficult to totally cure, it is in fact of Karmic nature and what the patient is having to experience during the current period of his life.

The next part of the procedure is to dowse for the factor causing the degree of deviation in the mental body, by watching the position of the pendulum it can be seen that environmental stress is causing the problem, the card for environmental stress can be placed in 'factor slot' and with the switch on, the measurement can be checked and verified.

This procedure is followed by testing the Astral Body, then Physical Etheric and so on throughout the Chakra systems, each time noting on the analysis chart the degrees of deviation as shown and if the deviations are plus or minus.

Following the Subtle body analysis are the tests to find the degrees of the other remaining factors as per the sheet, starting with the degrees of miasms affecting the patient, this is done by placing the All Miasms card in the factor slot with switch on the "on"

position, and measuring with the pendulum the degree of Miasm effecting the patient, noting the degree on the sheet.

The next part of the Analysis is the physical form, using the following sequence, and the question "what is the degree of deviation from functional perfection of the Aural system", with the mean-max switch at mean, make a note of the degree obtained, then first switch to 'max' and ask the question "the degree at worst point" and note the next reading.

This sequence proceeds through each physical system from Aural to Tonsils. When this is done the picture of the patient is complete, and will show a comparison of the subtle body energy deviations and the correspondent symptoms in the physical body. Now the treatment chart replaces the Analysis chart, for now is the time to search for a treatment against the main causative factor and location, this is done by placing the patient's sample on the treatment chart and asking for the treatment required in eradicating Enviromental Stress in the Mental Body, the pendulum will show the type of treatment required.

This could be any of the treatments shown on the chart, lets assume it is a colour we can then ask for the initial letter of the colour and then by placing the colour card in the correction slot and holding the pendulum at the degree of Enviromental Stress in the Mental Body, switch on the correction switch and if the treatment card is correct the pendulum will return to zero on the scale 7. To ascertain the potency the sweep dial is slowly turned anticlockwise whilst the pendulum is swinging along the zero line, when the pendulum begins to move away from zero it indicates that the optimum potency has just been passed, by a short turn clockwise the pendulum will swing along the zero line once again, this means that the potency indicated by the sweep dial position is the exact correction to eliminate the detrimental effects of the enviromental stress in the mental body. This basic proceedure is repeated for the worst degree of deviation in the chakra system and the worst point in the physical body.

This method of Analysis using the procedures on the subtle analysis sheet will give a full and detailed picture of your patient and the corrective measures necessary an experienced practitioner will complete the process in 25 - 30 minutes.

For Health care professionals wishing to ascertain the causative factor behind the anomaly affecting their patients, a simpler and faster but less detailed analysis can be used as follows:-

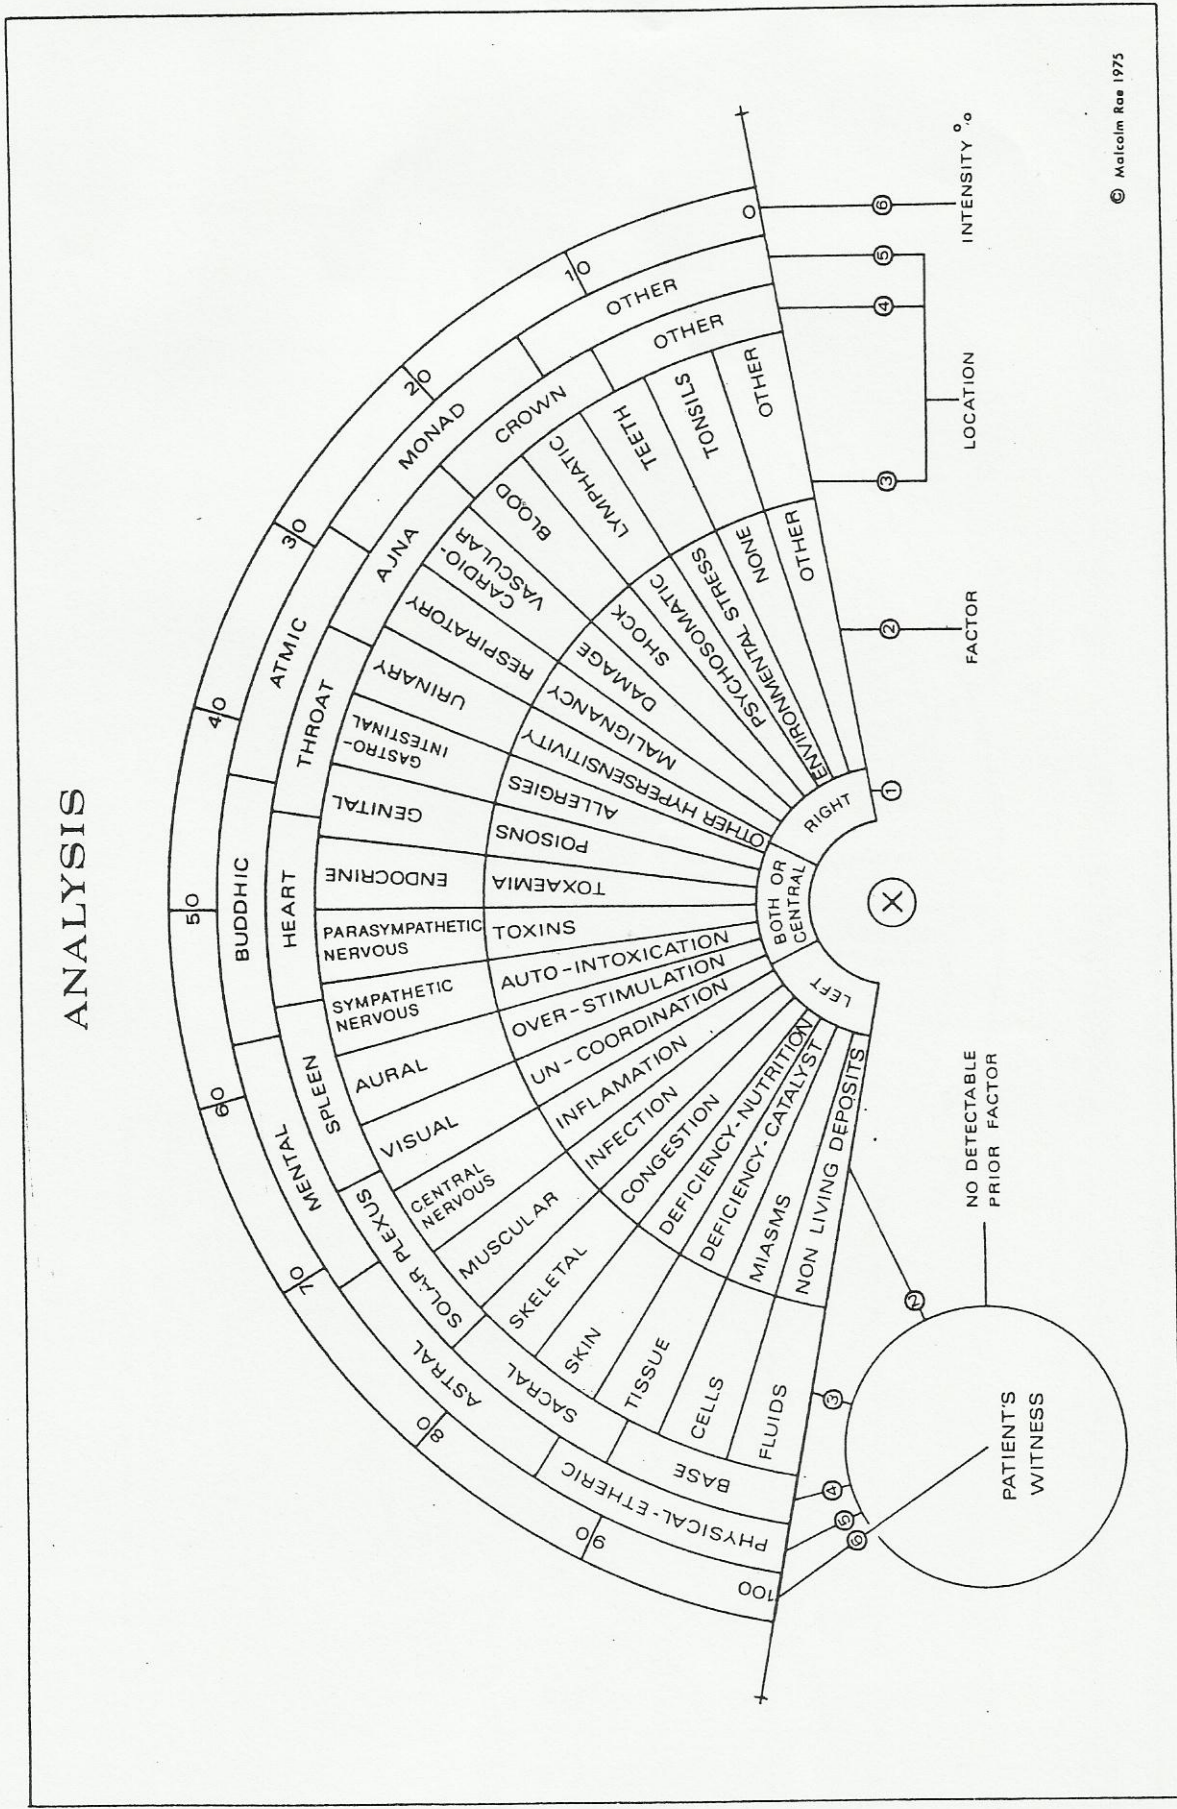


Fig. 19

10 Continue to repeat this series of operations until the pendulum, centred over the patient's witness, indicates "No detectable prior factor". At this point the combination of Factor and Location (e.e., "Congestion in the Physical-Etheric body) is the primary disorder, for which a remedy should be sought.

TREATMENTS FOR MRS JANE SMITH - AS PER SUBTLE ANATOMY ANALYSIS

- 1) Yellow, Potency 1M to the T.B. Miams Mental Body Base Chakra - 1 dose only.
- 2) Emerald Green, Potency 1M to Astral Body Head Chakra - 1 dose.
- 3) Dr. Bach combination of Rock Water/Olive/Impatiens orally - 4 times a day for 1 week.
- 4) Homoeopathic Ignatia 6x for 3 days - 2 day break followed by Homoeopathic Gelsemium 6c for 1 week.

General notes for patient:-

The reason for the mental body congestion and blockage is the patient's way of life blocking out the spiritual energies streaming from the Atmic area of the Spiritual Triad.

The patient should listen to the dictates of these energies and think less of materialism. She should be made to think of the higher aspects of life and be less inclined to dwell in the dense physical.

This would allow Base Chakra to respond and normalise, hence reflecting a healthier physical body.

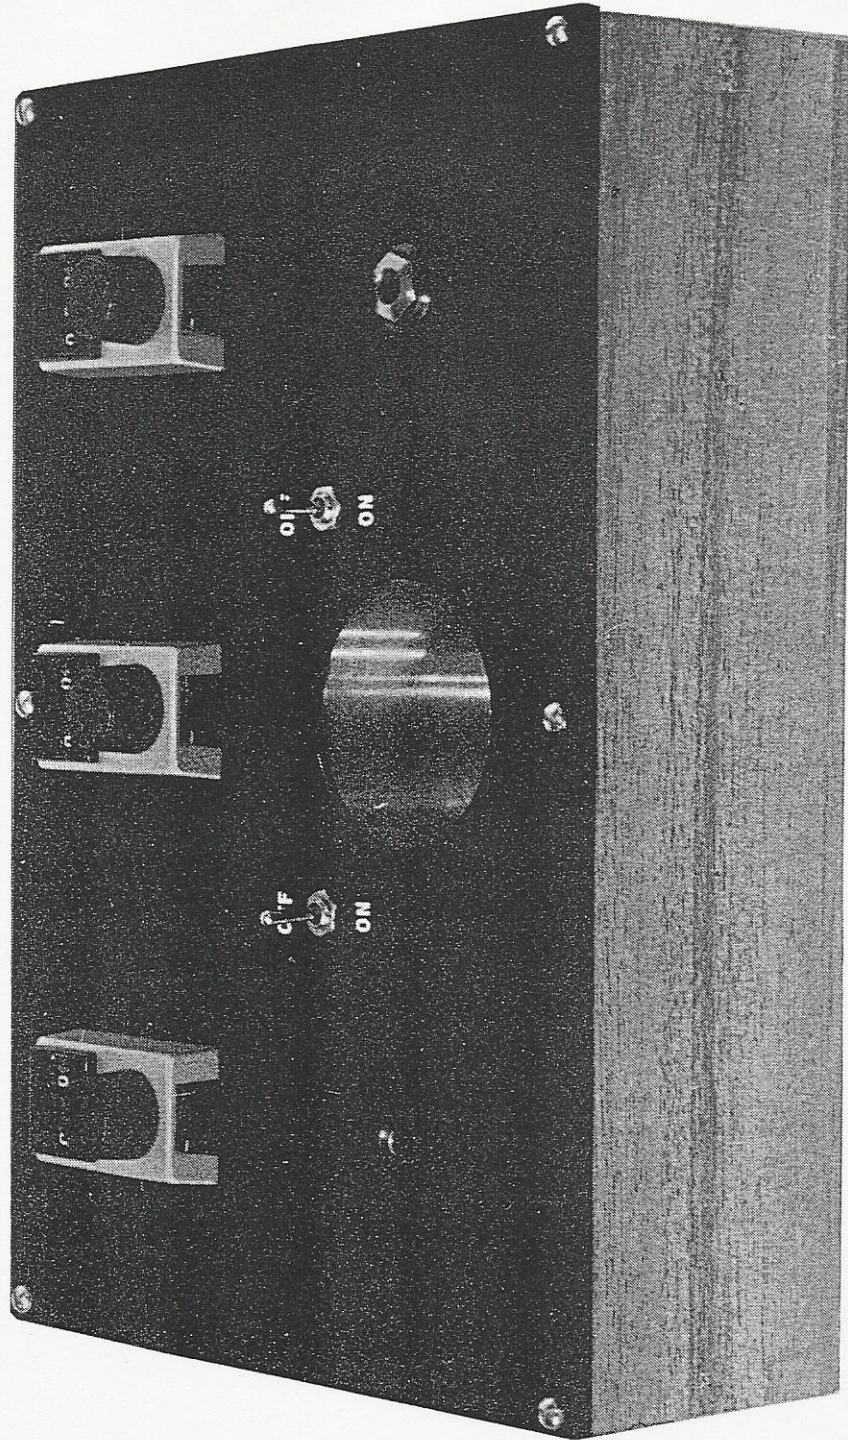


Fig 23. The Remedy / Factor / Location Instrument

THE TWIN AND TRIPLET INSTRUMENT

These instruments were designed for practitioners using the homoeopathic therapy with M.G.A. cards and evolved from many successful experiments that proved a label or additional information can be contained within the sac - lac pillules so potentised i.e. Homoeopathic Chelidonium can contain the vibratory rate of the liver to which it is directed.

The Triplet instrument may be used for single card potentising, twin usage or as many practitioners now use colours or gems directed to the energy centre and the organ or gland it controls i.e. Emerald Green to Sola Plexus Chakra to Pancreas.

Both of these instruments may be connected to the interrupter and so project the information across the patient's hair sample, or sac - lac may be potentised to be administered to the patient orally.

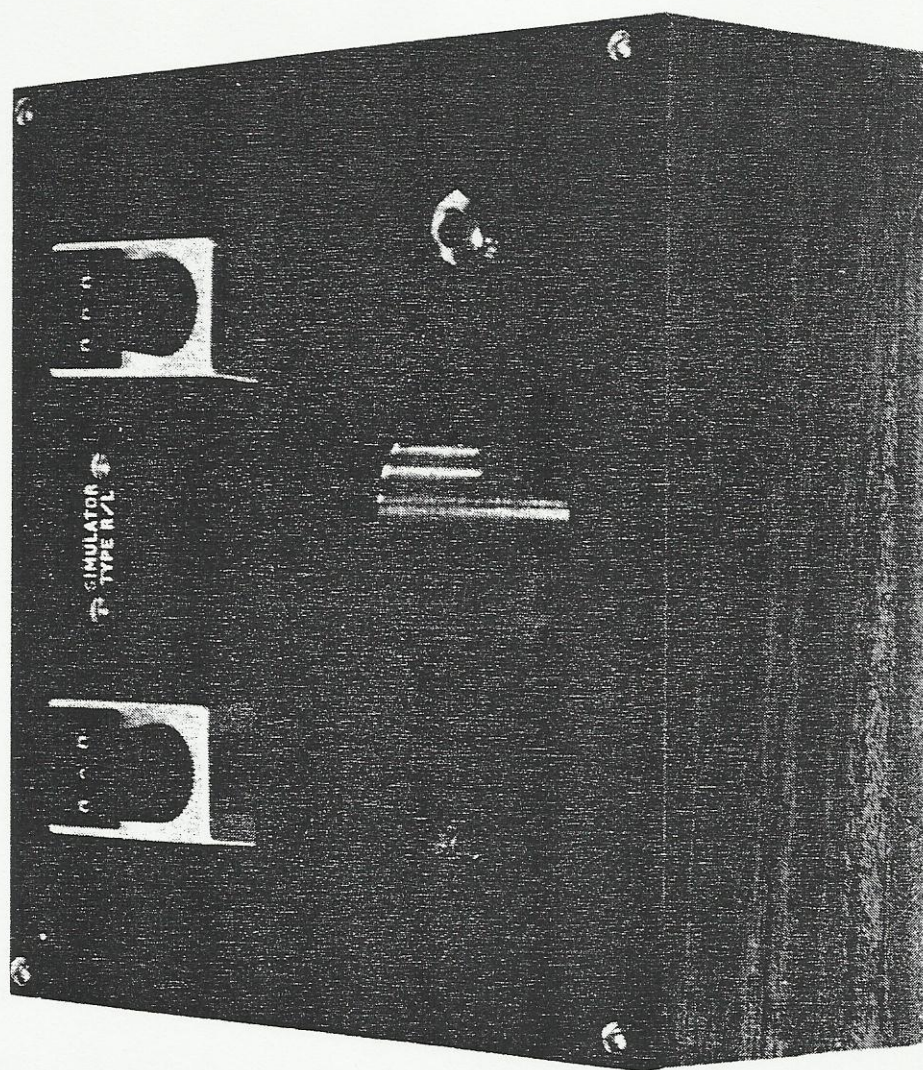


Fig 22 The Remedy / Location Instrument

SUGGESTED READING

Report on Radionics

By Edward Russell

Published by Neville Spearman Ltd

The Pattern of Health

By Dr. Aubrey Westlake

Published by Shambala

The Loom of Creation

By Dr. Dennis Milner & Smart

Published by Neville Spearman Ltd.

Radionic and the Subtle
Anatomy of Man

By Dr. David Tansley

Published by Health Science Press

Radionics Interface with
the Ether Fields

By Dr. David Tansley

Published by Health Science Press

Dimensions of Radionics

By Dr. David Tansley

Published by Health Science Press

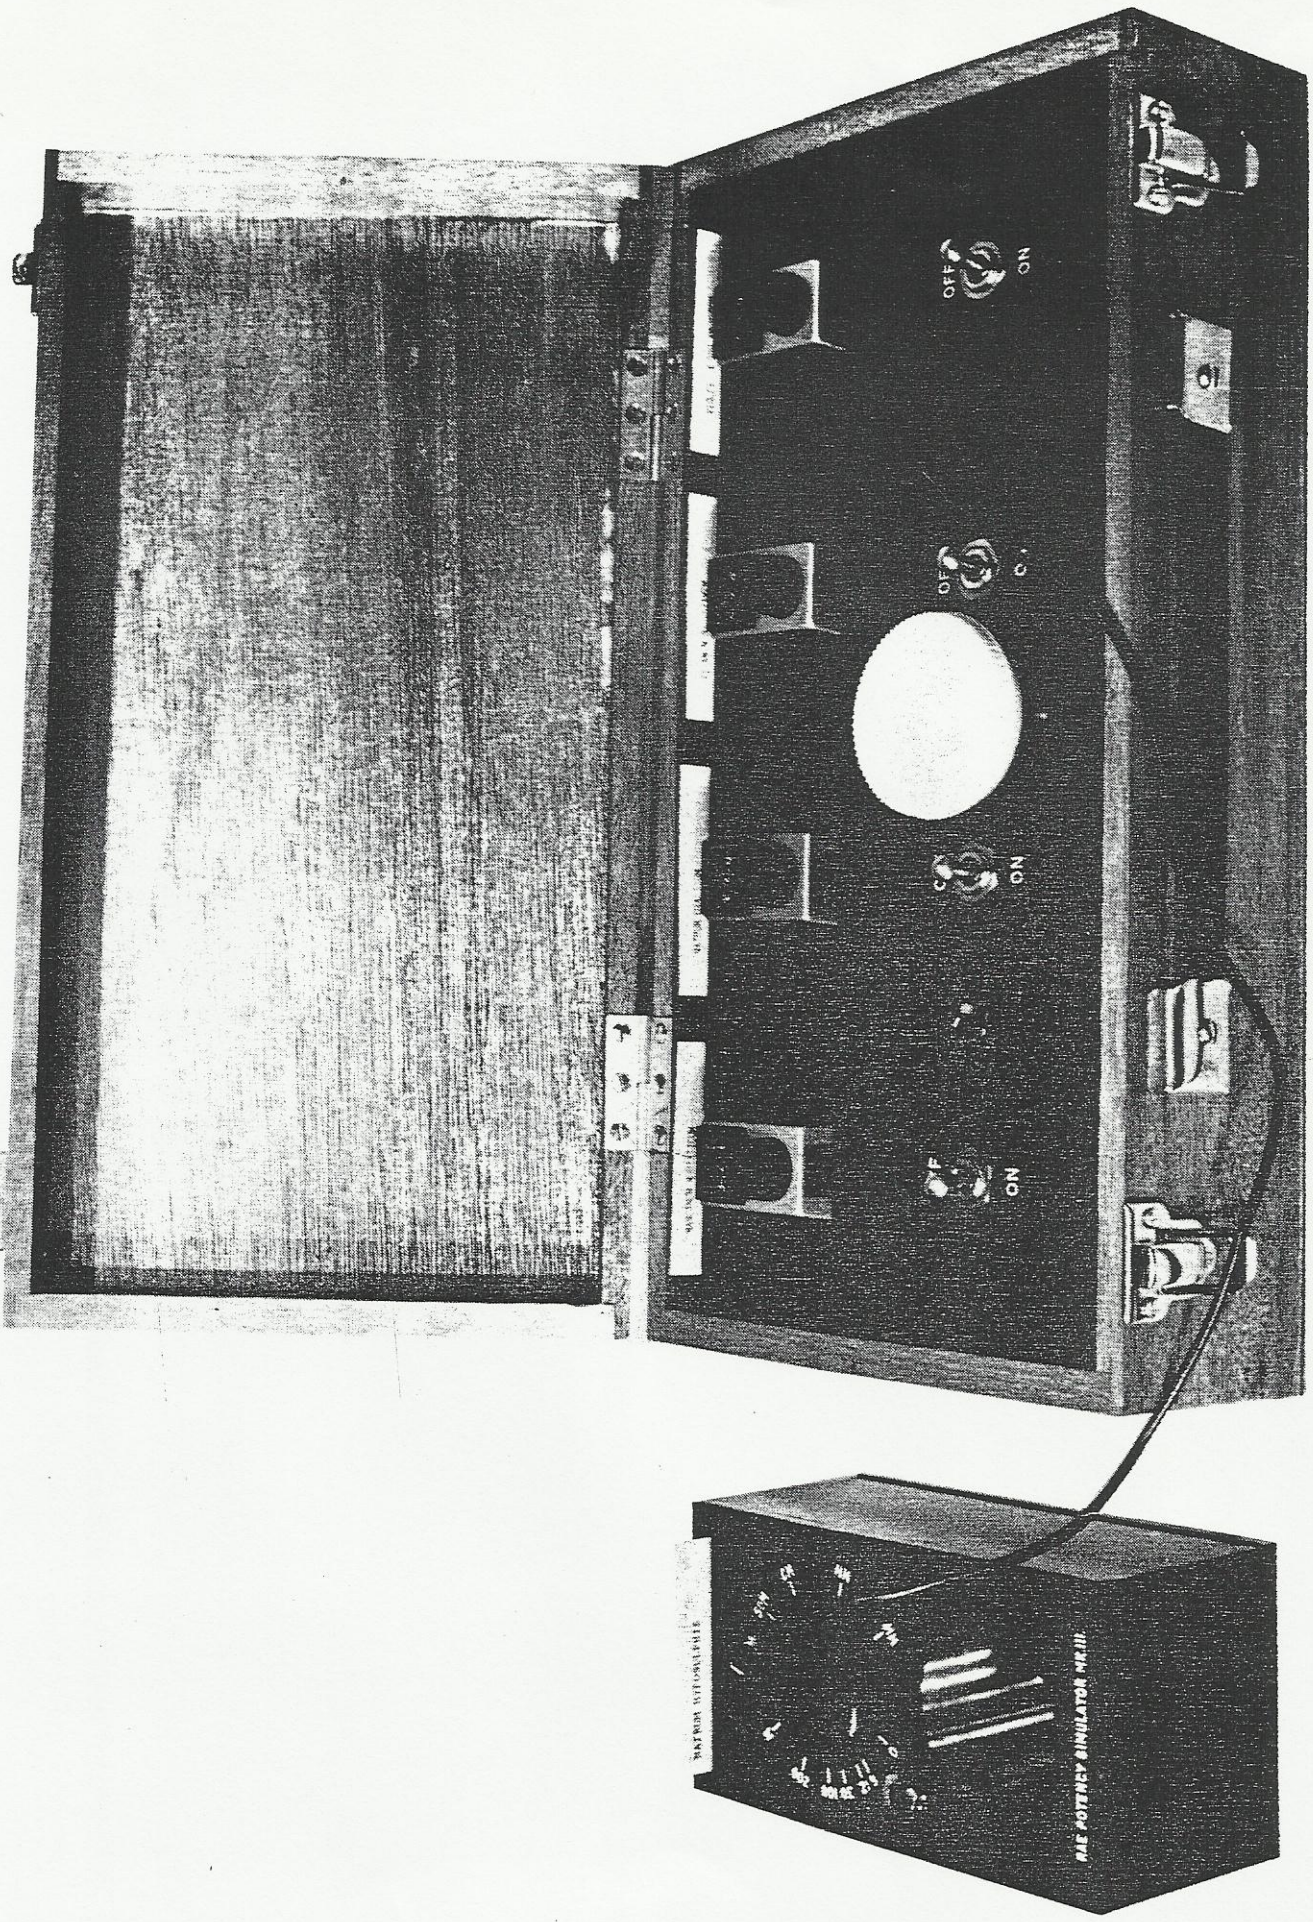


Fig. 24 A Potency Simulator connected to the Extended Range Multiple Potency Simulator

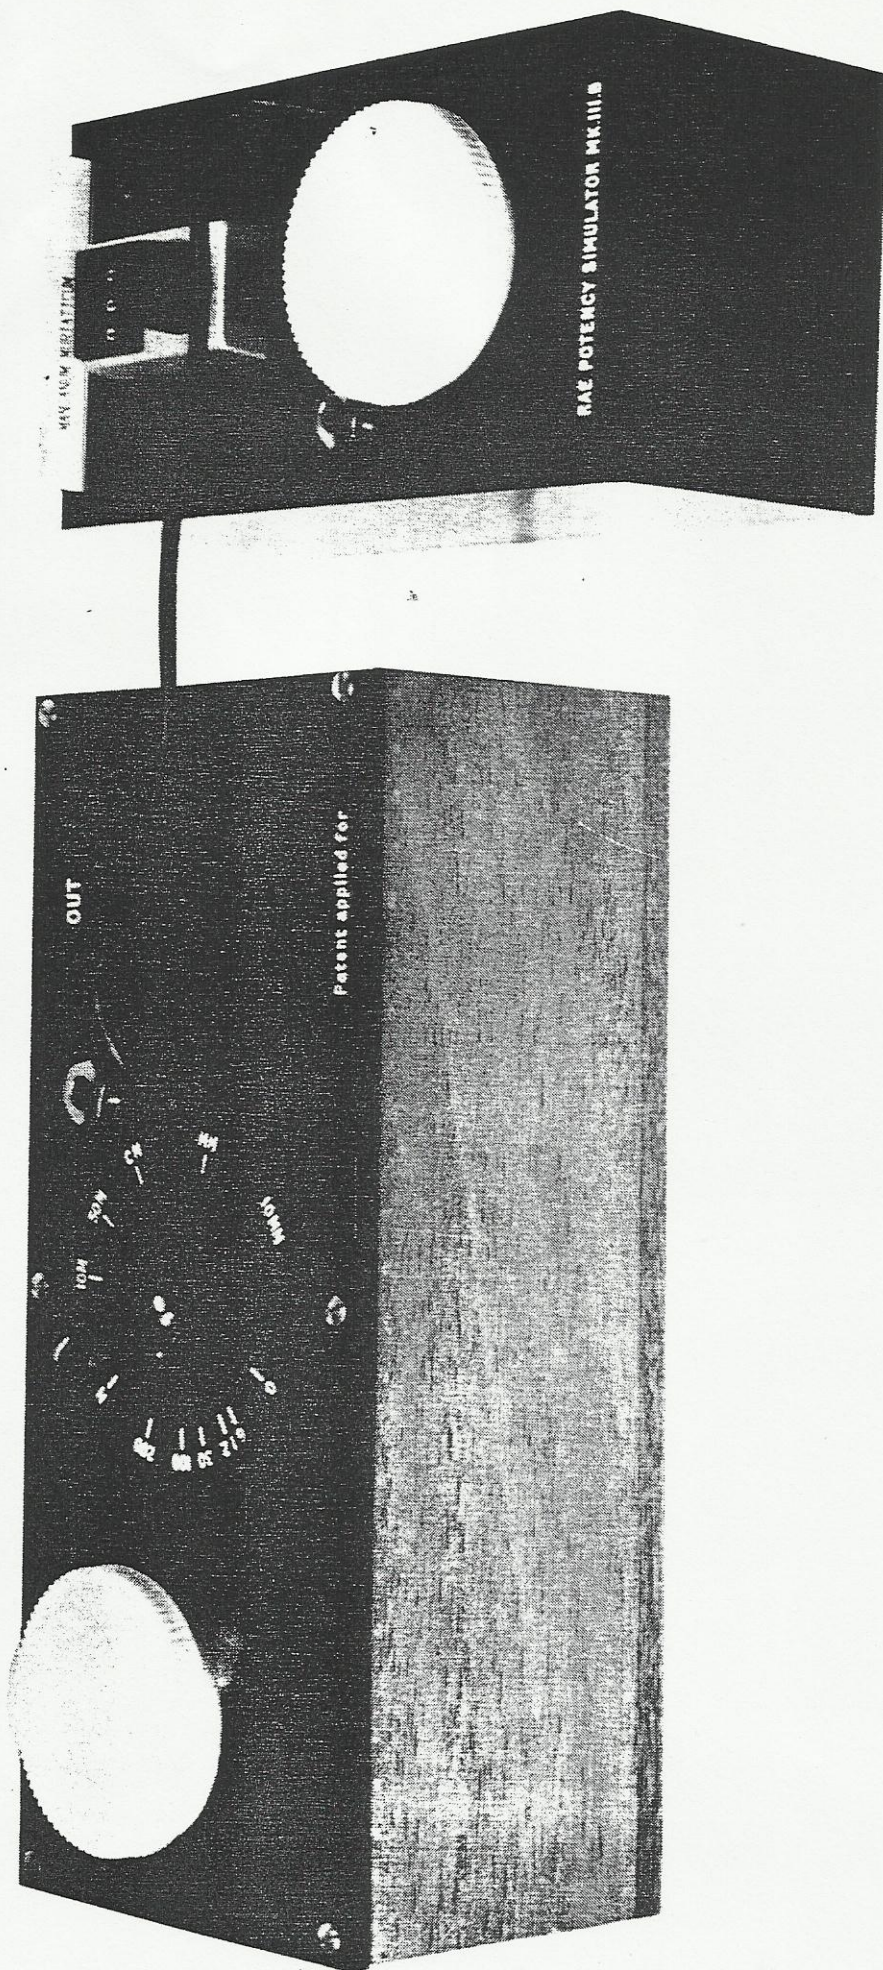


Fig. 25 A Potency Preparer connected to The Extended Range Potency Simulator